

CONTENTS

MANUAL i-health ENERGY SKIN CARE MODULE V5.0	1
CONTENTS	2
1. THE ENERGY SKIN CARE MODULE: SKIN REGENERATION BASED UPON EDA (ELECTRO DERMAL ASSESSMENT)	3
1.1 INTERACTIVE AND integrATED TREATMENT PROGRAMS	3
1.2 MERIDIANS AND ORGANS	3
2. THE ENERGY SKIN CARE MODULE: SUMMARY OF TREATMENT OPTIONS	5
2.1 computer generated cosmetiC interventions	5
2.2 treatment with the i-LIGHT and the i-MATRIX	6
3. HOW TO MAKE THE PROPER PROGRAM CHOICES	10
3.1 When to apply which program?	10
3.2 Contra-indications	12
4. TREATMENT SEGMENTS IN DETAIL	12
4.1 connective tissue treatment	12
4.2 Lymph drainage and connective tissue massage	14
4.3 Revitalisation /regeneration	14
4.4. Localisation of facial zones	14
4.5 Elimination through abdomen and thorax	17
4.6. Consolidation	17
4.7 STARTING UP THE ENERGY SKIN CARE-PROGRAM	18
5. THE PROGRAMS IN DETAIL	21
5.1 SKIN CARE I: GENERAL REGENERATION - DETOX OF CONNECTIVE TISSUE AND LYMPHATIC SYSTEM	21
5.2 SKIN CARE II: FACIAL REGENERATION - DETOX AND REVITALISATION OF FACIAL ZONES	21
5.3 REJUVENATION PROGRAM	21
5.4 ANTI-WRINKLE PROGRAM	21
5.5 ACNE PROGRAM	21
5.6 CELLULITE PROGRAM	21

5.7 SPECIAL SOLUTIONS _____	21
5.1. REGENERATION PROGRAM I _____	22
5.2 SKIN CARE II: FACIAL REGENERATION –DETOX AND REVITALISATION OF FACIAL ZONES _____	27
5.3 REJUVENATION PROGRAM _____	33
5.4 ANTI-wrinkle PROGRAM _____	39
5.5 ACNE PROTOCOL _____	47
5.6 CELLULITE PROGRAM _____	53
5.7 SPECIAL SOLUTIONS _____	59

1. THE ENERGY SKIN CARE MODULE: SKIN REGENERATION BASED UPON EDA (ELECTRO DERMAL ASSESSMENT)

1.1 INTERACTIVE AND INTEGRATED TREATMENT PROGRAMS

The i-Health equipment and software for electronic skin resistance measurements has been integrated with a device for modulated galvanisation, rhythmic vacuum massage, stimulation with colour sequences and electromagnetic regulation of dermatomes, reflex zones and acupuncture points.

All steps in the programs have been automatized, but the indications showed by the programs are the direct result of the measurements. Comparison of the client's skin resistance graphs before, during and after the cosmetic intervention show the client's exact reaction to what is going on during the treatment. This approach ensures a very effective and up to date treatment result.

1.2 MERIDIANS AND ORGANS

The human body is an open system concerning the exchange of energy and information. The classic Chinese meridians are the communication channels for that energy and information. They are supposed to be the most ancient known regulation system within the organism. Its development starts in the embryologic stage with the formation of the blastomeres. Meridians are protein chains with super conductive properties, following these tissue structures. The electric resistance of these protein chains provides information about the organic condition, functions and regulating processes that have been related to these meridians. The itronic measurement current has a neglectable impact on the organs and the meridians.

MERIDIAN	ORGAN	EXAMPLES OF MERIDIAN-ORGAN-FUNCTION CORRELATIONS
Lung	Lung	Immune system, skin, gaseous exchange
Large intestine	Large intestine	Lymphatic system, elimination
Stomach	Stomach	pH regulation
Spleen-Pancreas	Spleen, Pancreas, blood	N. Vagus, Carbohydrate metabolism and pancreas
Heart	Heart and blood circulation	Emotional influences, cardiac blood supply
Small intestine	Small intestine	Enzymatic digestion
Bladder	Bladder	Urogenital system, sinuses, eyes, spine
Kidney	Kidney	Elimination of water soluble toxins, regulation of fluids
Circulation	Pericard and pineal gland	Blood pressure, arterial innervation, pericardium
Triple Heater	Pituitary gland	Endocrine system
Liver	Liver	Protein metabolism
Gallbladder	Gallbladder	Cholesterol and fat metabolism

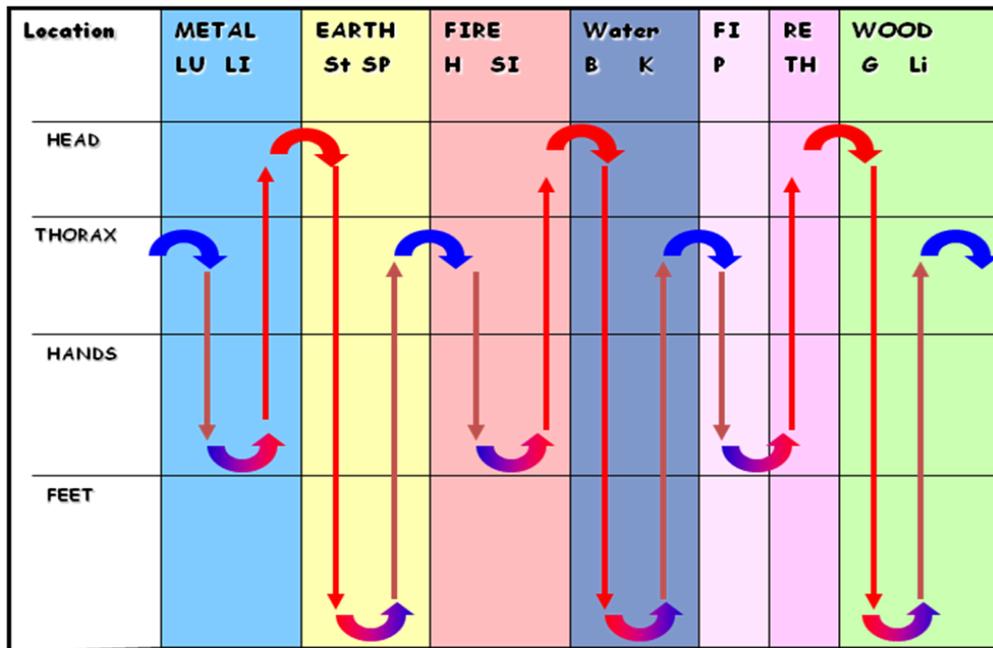


Fig. 2: Energy topography and polarity of the classic TCM meridian system. In the blink of an eye this picture shows the head area being totally Yang, the breast area being totally Yin, and the hands- and feet- area being energy polarity exchanging zones.

2. THE ENERGY SKIN CARE MODULE: SUMMARY OF TREATMENT OPTIONS

2.1 COMPUTER GENERATED COSMETIC INTERVENTIONS

- Assessment of vegetative stress, acidity and toxic accumulation by performing EDA at the distal meridian points on hands and feet, as described in TCM.
- Improvement of the vegetative stress regulation, stress capacity, regulation capacity, resistance, circulation of blood and lymph, detoxification, alkalisation and skin regeneration by means of electromagnetism, modulated galvanisation, vacuum massage technics and colour sequences.

The Energy Skin Care module is very versatile and flexible, providing a large range of treatment options.

This handout will explain:

- How the programs have been constructed
- Which regular TCM patterns have been applied
- How to find the similarities between the skin conditions of the client and the EDA energy profile
- How to make a logic and appropriate combination of the provided programs

In most cases, it is recommended to start with the Regeneration Programs I and II

2.2 TREATMENT WITH THE I-LIGHT AND THE I-MATRIX

2.2.1 THE HARDWARE.

Specifically developed and integrated instruments for the Energy Skin Module are the i-LIGHT (a very powerful LED-colour beamer) and the i-MATRIX: a compact device with a built-in vacuum pump (i-VAC), a galvanic modulator (i-ON) and a magnetic field generator. The i-VAC provides digitally managed rhythmic vacuum cupping on skin condition related connective tissue zones and lymphatic zones; the modulated galvanisation from the i-ON will be applied to dermatomes with a dermaroller and electrode rods. The magnetic field frequencies are applied to the body with a red Beamer.

The i-LIGHT battery can be charged with the 5 Volts-battery charger from the electric mains. Once the Skin Program has been started and both devices have been connected to the laptop, the appropriate Raymedies will be downloaded to the i-LIGHT by means of the USB-antenna.

The i-MATRIX device gets its power supply from the electric mains as well. The modulated galvanic and magnetic field signals are downloaded automatically by means of an antenna stick at the back of the device.

2.2.2. THE SOFTWARE.

The proper choice, order and treatment duration of the treatment signals, called "Raymedies", used during the cosmetic interventions are automatically indicated as a result of the EDA measurements. Just follow the instructions on the computer screen. The Raymedies are available in colour sequences, in modulated galvanic signals and in magnetic field signals. The colour sequences are applied with the i-LIGHT, the modulated galvanic signals with the i-ON and the magnetic field signals with the Beamer.

The Energy Skin Care module contains several programs, due to the actual personal cosmetic issues.

For example: the Energy Skin Care Facial Revitalisation program could be chosen. Just the first treatment with this protocol often brings already visible results. Besides that, specific programs are available for treating cellulite, acne, wrinkles, rejuvenation of face, neck and décolleté. "Special solutions" contains recently programs for couperose, micro-varicosis (Besenreisen), a special detox program and a demo-program. Other "special solutions" for contour-skin firming for breasts, arms, legs and buttocks, striae, moles, (de)pigmentations, couperosis, eczema, psoriasis are under construction

2.2.3 CONSTRUCTION OF THE PROGRAMS

All programs have similar construction and integrated technology and performance as both basic regeneration programs, but with a focus on specific problematic areas. In sessions between 60-90

minutes, the face, the spine, the belly, the breast and legs are treated in 4 subsequent steps, in a very pleasant, thorough and effective way:

1. Matrix regulation
2. Revitalisation/regeneration
3. Elimination
4. Consolidation

Especially this construction and integration of technology will take care of adequate stimulation of fibroblasts and collagen, which is necessary for revitalisation and skin rejuvenation, together with alkalisation, detoxification and improved circulation, to maintain the visible results.

2.2.4 MATRIX REGULATION

In Regeneration Program I detoxification preparations are made in the connective tissues. This system is also called the Matrix, the BBRS (Basic Bio Regulation System) or Pischinger's Basic System.

The connective tissue system controls the maintenance of homeostase, which is the internal biologic balance by continuous adaptation to external changing circumstances. Homeostasis ensures the stability of vital functions like temperature, blood pressure, blood sugar level, immunity and pH. In many situations, the connective tissue system has been polluted. In order to promote detoxification and facilitate homeostasis, specific organic dermatomes will be treated in an integrated way. An important and effective access to these dermatomes are the so-called Back-Shu- or YÜ-points along the spine, on the inner branch of the Bladder meridian. The proper choice of those points is automatically made by the program, as a result of previous EDA measurements. The table below shows the correlations between the YÜ-points, organs, dermatomes and their localization. The several colours of the points in the picture are according the 5 elements: Metal (B13 and B25) silver gray, Wood (B18 and B19) green, Fire (B14,15,22 and 27) red, and Water (B23 and B28) blue.

NAME	ORGAN	ELEMENT	CONNECTIVE TISSUE ZONES	LOCATION
B13	Lungs	Metal	Lungs, bronchi, pleurae, breast	ICR 3
B14	Pericard	Fire	Gallbladder, stomach and spleen	ICR 4
B15	Heart	Fire	liver, stomach, solar plexus and blood	ICR 5
B18	Liver	Wood	adrenals	ICR 9
B19	Gallbladder	Wood	Kidneys, intestinal and vascular walls	ICR 10
B20	Spleen/pancreas	Earth	Kidneys, bladder, urethra, prostate	ICR 11
B21	Stomach	Earth	Small intestine, ovaria, lymph circulation	Below 12 th rib
B22	Triple Heater	Fire	Colon, groins	Between L1 and L2
B23	Kidneys	Water	Appendix, lower belly, upper legs	Between L2 and L3
B25	Large Intestine	Metal	Prostate, lower legs, ankles, feet, toes	Between L4 and L5
B27	Small Intestine	Fire	Hips, pelvis, buttocks	Next to lower edge of S1
B28	Bladder	Water	Hips, pelvis, buttocks	Next to lower edge of S2



The Matrix-regulation will take place in 3 steps:

- a. Frequency modulated phoresis with the **i-ON** -dermaroller brings a direct current in the body on zones and with frequencies, selected by the body itself as a result of previous EDA-measurements. Most of these problem-related dermatomes have been localized in the face, along the spine and in the abdominal areas. Treating these dermatomes will support circulation, detoxification, alkalization, and *“last but not least”*: remarkable strengthening, rejuvenation and improvement of facial skin and connective tissue elasticity by stimulation of natural manufacturing of fibroblasts.

- b. Thereafter, homeostasis will be supported powerfully by the ***i-MATRIX***: rhythmic, deep vacuum cupping will activate cellular metabolism, lymphatic and capillary circulation, will remove subdermal adhesions and lumps, and will regulate the autonome nervous system by vegetative feedback to and from the treated dermatomes.
- c. All problem-related spinal segments will be treated, from head to buttock area. Energetic constitution related essential oils will enhance the treatment result.
- d. Finally, the same selected dermal segments will be radiated with the ***i-LIGHT***. This very powerful LED-color beamer will create photo modulation of the mitochondria and DNA-synthesis, and photon transport by cells, skin-, connective tissue and muscles. Power supply of all these organisms will be re-established literally. Flexibility, firmness and gloss of skin will benefit from this in a visible way. Besides stress regulation, the i-LIGHT treatment result is harmonizing, relaxing and revitalizing. Contra-indications are histories of convulsions and direct exposure to the eyes.

2.2.5 FACIAL REGENERATION/REVITALISATION: “THE GALVANIC FACELIFT”.

Regeneration program II starts with the treatment of de cervical spine, subsequently with the i-ON, the i-VAC en the i-LIGHT. This treatment obliquely activates the facial dermatomes. The three preceding measurements are necessary to select the facial dermatomes corresponding to the weakest meridian, and to select the correlating frequency signals in order to perform a direct “galvanic facelift”.

Improvement of alkalization, detoxification, circulation and elasticity will now be executed on the problematic facial zones themselves, with the i-ON-dermaroller and the rod electrodes.

Thereafter, the whole face and neck will be massaged with the vacuum cups of the i-VAC. Lymphatic drainage and connective tissue massage is achieved by adjustable suction power and pulse frequency, together with energetic constitution related essential oils.

Finally, photonic distribution and stimulation of facial DNA synthesis will be activated by the i-LIGHT color sequences that are corresponding to the weakest meridian.

2.2.6 ELIMINATION: CONNECTIVE TISSUE- AND LYMPH DRAINAGE OF ABDOMINAL AND THORACIC ZONES

Specific abdominal and thoracic elimination zones will be treated with the i-VAC cupping techniques as well, together with personalized complexes of essential oils. Preceding measurements are necessary to establish the proper directions of movement during these procedures.

- In case of energy-excess of the constitutional element, downward moving techniques will be dominating.

- In case of energy depletion or normal energy of the constitutional element, upward moving techniques will be dominating.

2.2.7 CONSOLIDATION WITH MAGNETIC FIELD FREQUENCIES AND INFRARED

The last step in each treatment program enables the client to respond to all the effects of matrix regulation, facial revitalization and elimination in terms of post-vegetative regulation. A final EDA measurement will show the total treatment effect on the client so far. The program will calculate the most adequate magnetic field signal to facilitate an optimal post-vegetative regulation.

That specific regulating signal will be applied with the red Beamer (the EM-transmitter) to the thoracic, abdominal or neck region. As a result, capillary and peripheral circulation will be balanced, as well as cellular and neurotransmitter metabolism, creating a deep and very pleasant feeling of relaxation and tranquility.

3. HOW TO MAKE THE PROPER PROGRAM CHOICES

3.1 WHEN TO APPLY WHICH PROGRAM?

In most cases, it is recommended to start with Regeneration Program I (General Detox), to continue with Regeneration Program II (Facial Revitalization) after one week.

Besides that, the Energetic Skin Care Module contains specific programs for Cellulite, Wrinkles, detoxification, Rejuvenation, Acne, and "Special Solutions" for conditions like couperosis/rosacea and micro-varicosis (Besenreisen). All programs contain the same construction and integration of technology, taking care of the proper reactivation and free energy flow by removing acid, toxic, stagnated and accumulated energy. As a result, the body will react in terms of:

- Improved repairing skin capacity
- Enhanced cellular activity and -metabolism
- Stimulation of natural fibroblast manufacturing
- Improved moisturizing skin capacity
- Improved skin metabolism and circulation
- Improved skin surface (smoother, more elastic, more glossy)
- Improved connective tissue structure
- Fading of facial lines and deep wrinkles

- Refinement of skin pores
-

TABLE OF PROGRAM OPTIONS

SKIN CONDITION	POSSIBLE CAUSE	WHICH PROGRAM?
Dry and scaly skin	Insufficient management of fluids and waste	Regeneration program I and II Rejuvenation
Tight and tearing skin	Lack of fluids and moisture	Regeneration program I and II Rejuvenation
Blemishes and irritated skin	Lack of protection, enhanced pH, poor balance moisture and fat verhouding vocht en vet	Regeneration program I and II Rejuvenation
Sallow skin	Poor circulation	Regeneration program I and II Rejuvenation
Poor healing capacity	Decreased fibroblast activity	Regeneration program I and II Rejuvenation
Wrinkles in general	Discongruence of cellular layers	Regeneration program I and II Anti-wrinkle
Prominent nose-mouth wrinkle	Withered moisturizing of cheeks, decreased elasticity	Regeneration program I and II Rejuvenation Anti-wrinkle
Rings around the eyes	Decreased elimination of waste, decreased supply of oxygen and nutritives	Regeneration program I and II Rejuvenation
Forehead wrinkles	Cracks and adhesions of connective tissue	Regeneration program I and II Rejuvenation Anti-wrinkle
Frown wrinkles	Adhesions of skin layers	Regeneration program I and II Anti-wrinkle
Wrinkles on cheeks	Cracks and adhesions of connective tissue	Regeneration program I and II Rejuvenation Anti-wrinkle
Couperosis	Vascular capillar sclerosis	Regeneration program I and II Couperosis Rejuvenation
Irregular pigmentation	General deterioration of skin condition and imbalanced fat/moisture ratio	Regeneration program I and II Rejuvenation
Upper lip wrinkles	Lichnification	Regeneration program I and II Rejuvenation Anti-wrinkle
Acne vulgaris	Androgene hormones, imbalanced metabolism, bacterial infections, external circumstances	Regeneration program I and II Acne

Cellulite	Hormones, accumulation and adhesion of fat cells, moisture and toxins	Regeneration program I and II Cellulite
-----------	---	--

3.2 CONTRA-INDICATIONS

Some conditions or circumstances are not suitable for the whole energy skin care approach, or parts of it, such as:

- Burns, scalds, open wounds
- Skin infections or inflammations, viral en bacterial skin diseases
- Boils and other kinds of contagious skin eruptions
- Serious organic and/or contagious diseases
- Electromagnetic stimulation is a contra-indication for pregnant clients, clients with increased chance of thrombosis, clients with pacemakers, implanted defibrillators, or implanted hearing aids
- No i-LIGHT exposure in faces of clients with a history of convulsions

4. TREATMENT SEGMENTS IN DETAIL

4.1 CONNECTIVE TISSUE TREATMENT

4.1.1 INTRODUCTION

The connective tissue system is in fact our largest organ. Together with extracellular fluids, it contains more than 60% of all human tissues. It interconnects the skin, muscles, fat, fluids, cells and organs. As an independent system, it is called B.B.R.S.(Basic-Bio-Regulation System), the Matrix, or Pischinger's System.

This system regulates all vital functions like respiration, circulation, energy management, metabolism, temperature and pH.

It also controls the permanent exchange between the Autonomic and the Central Nervous system, the Endocrine system and the Immunity system.

Distributors of that huge and complicated exchange are neurotransmitters and metabolic, immune regulating and endocrine substances. All primal counter measures against pathogenic factors like cold, wind, heat, damp, moisture, infections, injuries, scars, alien substances are taken within the connective tissue system.

Life style, habits and life circumstances, attitude to life, and nutrition play an evident role in maintaining efficiency of this autonomic self-regulation and adaptive capacity.

Biochemical pollution of the connective tissue system by permanent overload seems to be one of the most important causal factors in chronic illnesses.

That's why thorough and consequent detoxification of the connective tissue system is the first and best step on the way back to vitality, beauty and health.

4.1.2 CONNECTIVE TISSUE ZONES: AN INTEGRAL TREATING AREA

Chronic changes of the connective tissue, caused by permanent disregulation can be observed in certain dermal zones by discolorations, differences in structure, temperature, circulation, and tissue retractions. These dermal zones are related to internal organs by segmental innervation.

The relationship between certain internal organs and (sub)dermal zones has been discovered around 1900 by the English neurologist Head. That's why these connective tissue zones are mentioned "Head's zones".

All internal organs and functions have their own projection area in connective tissue zones, right under the skin. Treating these connective tissue zones in an integrative way will facilitate the self healing capacity of all related body parts in an hormonal, neurological and immunological way.

4.1.3 THE GENESIS OF CONNECTIVE TISSUE ZONES

Embryological development is in fact a segmental construction: a successive range of joined "slices" with similar compositions. These "slices" are called "somites", and contain different structures. These structures are the sources of specific tissues, which are formed in a later stage of development.

Sclerotome the formation source of bone tissue

Myotome: the formation source of muscular tissue

Dermatome: the formation source of skin tissue

Vasotome: the formation source of blood vessels

Viscerotome: the formation source of internal organs

Neurotome: the formation source of neural tissue

One particular segment contains all these structures, which makes it comprehensible that each particle of skin, muscle, bone, nerve, vessel or organ originates from a spinal segment.

4.2 LYMPH DRAINAGE AND CONNECTIVE TISSUE MASSAGE

Lymph drainage and massage of the entire connective tissue system will take place with vacuum cupping techniques with specific rhythmic changing suction ("i-VAC"). This promotes vascular circulation, extracellular metabolism, the returning lymphatic circulation and the interstitial discharge of toxins, causing a deep and thorough cleansing of all tissues and the entire skin.

Premature and accelerated ageing will be slowed down significantly by systematic and integrated application of lymph drainage and connective tissue massage, together with "galvanic facelifting", colour therapy and electromagnetic field therapy. That's why each client feels very relaxed and fit after any energy skin care treatment.

4.3 REVITALISATION /REGENERATION

Indirect alkalization, improvement of circulation and elasticity is the result of treating facial zones with the i-ON

Lymph drainage and connective tissue massage of face and neck will be executed with the i-VAC.

Concluding treatment of the face with the i-LIGHT promotes stimulation of photonic distribution and DNA synthesis by application of specific skin revitalizing color sequences.

4.4. LOCALISATION OF FACIAL ZONES

UPPER HORIZONTAL FOREHEAD ZONE, NEXT TO THE HAIR OF THE HEAD

This zone has been related to Bladder energy. Horizontal wrinkles with a scaly and dry skin may be the result of stagnated fluids by weakened kidney- and bladder energy.

MIDDLE HORIZONTAL FOREHEAD ZONE

This zone has been related to the small intestine. Poor digestion by enzymatic problems are often the result of incomplete elimination of waste and toxins, causing wrinkles and pimples in this area. Excretion and elimination can be improved and facilitated by nutritional corrections, more physical activity and drinking more natural water. Besides hereditary factors, too much ploddering caused by chronic problems with making choices and setting priorities may cause premature wrinkling in this area.

A pale or red forehead may indicate upset vascular circulation or emotional imbalance.

TEMPORAL ZONES

This zone has been related to the gallbladder. Skin eruptions here may indicate accumulation of fatty waste and possible frustrations due to too high expectations and impatience.

ZONE BETWEEN THE EYEBROWS

This zone has been related to the liver. Vertical wrinkles here may indicate excessive eating and drinking, chronic stress, lack of healthy sleep, and emotional imbalance by unexpressed feelings of general inability.

ZONE AROUND THE EYES

The area below the eyes has been related to the kidneys. Black-blue eye rings may indicate poor kidney- and bladder energy. These dark rings are often hereditary and may show dehydration, accumulated fluids and a poor excretion of fluids. The area above the eyes has been related to the spleen/pancreas energy. Stagnated fluids here may indicate problems with carbohydrate- and sugar metabolism. Yellow brown fat accumulation around the eyes may indicate chronic problems with gallbladder and liver functions. Grey colored eye zones may indicate exhaustion, stress and disturbed vascular circulation..

NOSE

The nose has been connected to the lungs, hence respiration.

The nose tip and nose bridge have been related to the heart energy. A red nose with diluted capillary vessels may indicate a vascular problem, possibly related to blood pressure and chronic nutritional problems.

NOSTRIL-MOUTHCORNER-FOLD

This zone has been related to the large intestine. Skin eruptions or a deep crease along the nostrils may indicate accumulated waste and toxins, caused by deficient colonic activity (constipation or dysbiosis).

CHEEKS

Wrinkles in the jaw bone area may indicate imbalanced lung energy. The part just above the jaw bone, but below the kidney zone, belongs to the stomach.

Sensitive red couperosis cheeks may be the expression of imbalanced lung-, stomach-, spleen- and/or heart energy. Slight swellings may be an indication of disturbed colon energy

ZONE AROUND THE MOUTH

The skin around the mouth is related to the circulation meridian.

Vertical wrinkles around the mouth may indicate hormonal problems.

Pimples and sores in the corners of the mouth may indicate disturbed heart energy and/or colon energy.

CHIN

This zone, together with the eye zones, is related to the kidneys. Inflammations and obstructions may indicate accumulated waste in the kidneys, poor circulation of fluids and menstruation problems. Skin troubles like excessive hair growth may be correlated to hormonal disbalance; impurities in the skin zone may also indicate poor intestinal functions.

LATERAL JAW CORNER

This zone is related to the gallbladder energy.

NECK

Red spots or an impure skin with pimples is often related to the stress hormone cortisol. Skin eruptions in the neck or breast area are often related to an emotional disbalance and problems with lungs and vascular circulation.

TABLE FACIAL ZONES

FACIAL ZONES	LOCALIZATION	RAYMEDY
Bladder zone	Upper horizontal area of forehead	Renastimutron
Kidney zone	Area below the eyes and Chin area	Renastimutron
Liver zone	Area between the eyes	Hepastimutron
Gallbladder zone	Temporal area Jaw angle area	Hepastimutron
Heart zone	Nose tip and nose bridge	Corstimutron
Small intestine zone	Middle horizontal area of forehead	Lienostimutron
Circulation zone	Area around the mouth	Thalastimutron
Triple heater zone	Lateral eyebrow angle	Corstimutron
Stomach zone	Cheek area just above the cheek-bone	Lienostimutron
Spleen zone	Area above the upper eye lids	Lienostimutron

Lung zone	Cheek-bone area, nostrils	Pneumastimutron
Large Intestine zone	Fold between nostrils and corners of the mouth	Pneumastimutron

4.5 ELIMINATION THROUGH ABDOMEN AND THORAX

Connective tissue massage and lymph drainage of the abdominal and thoracic zones with the i-VAC

4.6. CONSOLIDATION

The last step in each skin care program concerns the consolidation with magnetic field frequencies. This enables the client to enjoy a deep and very pleasant feeling of relaxation and tranquility while the body is responding to the overall treatment effect in finding a new equilibrium, a new homeostasis. The program will calculate the most adequate magnetic field signal to facilitate this, and shows where to apply this signal with the red beamer.

LOCALIZATION OF ACUPUNCTURE POINTS FOR CONSOLIDATION

JM-3	anterior midline, 1 cun above the pubic bone
JM-8	in the navel
JM-12	anterior midline, midway between the sternum and the navel
JM-17	anterior midline, at the centre of the breast bone
DM-14	posterior midline, just below vertebra C7 (neck-shoulder-level)

4.7 STARTING UP THE ENERGY SKIN CARE-PROGRAM

To obtain optimal synergistic results, it is recommended to start each energy skin care program with a radiation of the face with TDP infrared during 8 minutes.

THE TDP LAMP

According to recent scientific research, far infrared facial thermal therapy has a significant revitalizing effect on the facial skin. That's why we strongly recommend to start every future energy skin care treatment with a facial thermal treatment during 8 minutes, and the best way to obtain optimal synergistic results, is with a TDP lamp.

The TDP mineral lamp is a medical device which comes under FDA Class II as a far-infrared thermal therapy device. The lamp is NOT included in the hardware of the energy skin care program



While most lamps use a common near infrared bulb, the specially engineered TDP lamp emits a special band of far infrared electromagnetic energy (in the 2-50 micron range). This bandwidth is similar to the beneficial far-infrared radiation from hot clay applications as used in balneotherapy. Analysis of the clay and later experimentation led to the development of the medical device now known as the TDP mineral lamp, as a therapeutic substitute for moxabustion. The lamp also features a unique mineral plate which is coated with a proprietary mineral formulation consisting of 33 trace elements. These trace elements are also found in the human body, in various chemical binding forms. Because the human body has a higher absorption efficiency for far infrared energy than near infrared, possible insufficient amounts of human trace elements will be replenished. Clinical evidence confirmed that the combination of far infrared with trace elements emission increases microcirculation, balances metabolism, promotes specific enzyme activity levels, immune function, cell growth and repair, regenerates the skin and loosens connective tissue adhesions to accelerate the natural healing processes of the body.

TDP is an acronym for "Teding Diancibo Pu" which loosely translated means special electromagnetic spectrum.

The TDP mineral lamp was invented in China in 1978 and was patented in China in 1992

It is used by acupuncturists, Asian bodywork therapists, and other medical professionals. The state of research in 1985 showed TDP mineral lamp therapy to have been successfully used to treat over 30 different human and animal diseases and disorders.

In the U.S.A., TDP mineral lamp therapy has a billable modality number 97026 for doctors to bill insurance providers. The class of devices to which it belongs is approved by the FDA for temporary relief from pain and arthritis.

ADDED SYNERGISTIC COSMETIC PRODUCTS

We recommend 4 synergistic cosmetic products, that can be purchased online from FITLINE (online: www.907.pm-international.com or with telephonic support of Mrs. Itt from Luxemburg (00352 621 140 737)


- **RESTORATE** to remineralize and alkalize the treated skin areas
- **ACTIVIZE OXYPLUS**, improved oxygen supply and circulation
- **Q10 DROPS** to enhance cell regeneration, cell function, antiwrinkle and skin repair results
- **Beauty line 12h Active Serum** to optimize anti-wrinkle treatment
- **CC CELL LOTION** to optimize cellulite treatments, generates strong local hyperaemia and warmth

These products in combination with i-ON treatments showed such a remarkable synergistic treatment effect that we decided to integrate them in the treatment protocols.

Mix ratio's to be prepared for i-ON application:

- **All programs:** Aloe vera + Restorate (2 table spoons : 1 level tea spoonful)
- **Acne:** Aloe vera + Q10 (1 table spoon : 7 drops)
- **Rejuvenation, anti-wrinkle and special solutions:** Aloe vera + Q10 + Beauty line active serum (1 table spoon : 7 drops : 6 sprays)
- **Cellulite:** Aloe vera + CC Cell Lotion (1 : 2)+ 1 LTS Cinnamon+1LTS Activize Oxy Plus

The program itself always starts with 3 EDA measurements. By clicking the "CONTINUE"-arrow, the Skin Care Alkaline Balance introduction will appear on the screen, which is meant to be read by your client. It is recommended, to mail this introduction at least a week preceding your clients first consultation, to ensure a good preparation. By clicking again the "CONTINUE"-arrow again, you will enter the selection-menu of the energy skin module.

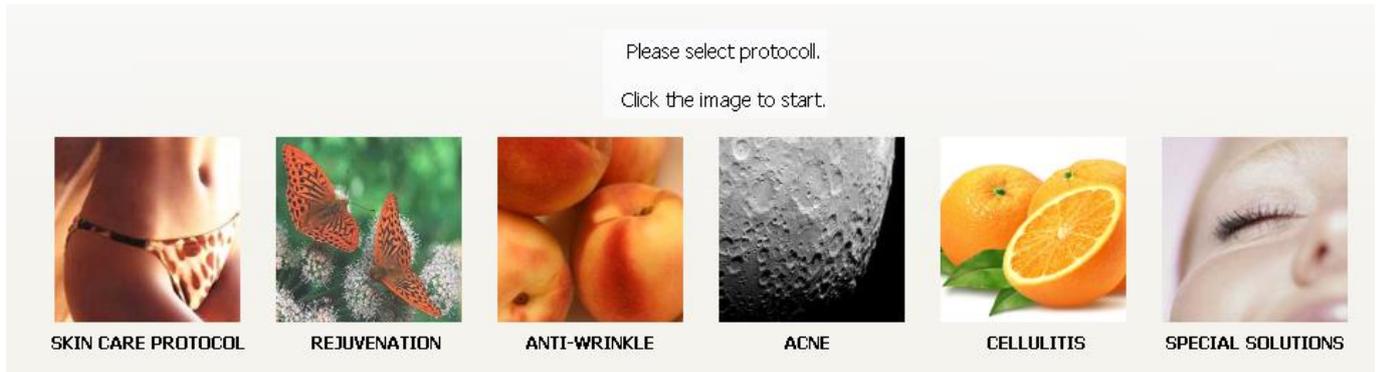

The left image is called "Skin care protocol". Clicking this image opens the next screen:

Indication of element-type, energy amount, name of weakest meridian

Option to select regeneration program 1 (general detox and regeneration) or 2 (facial revitalisation)

back continue

5. THE PROGRAMS IN DETAIL

5.1 SKIN CARE I: GENERAL REGENERATION - DETOX OF CONNECTIVE TISSUE AND LYMPHATIC SYSTEM

5.2 SKIN CARE II: FACIAL REGENERATION - DETOX AND REVITALISATION OF FACIAL ZONES

5.3 REJUVENATION PROGRAM

5.4 ANTI-WRINKLE PROGRAM

5.5 ACNE PROGRAM

5.6 CELLULITE PROGRAM

5.7 SPECIAL SOLUTIONS

5.1. REGENERATION PROGRAM I




SKIN CARE PROTOCOL

5.1.1 SKIN CARE I: GENERAL REGENERATION, STEP 1

This is the first step in matrix-regeneration. That means: modulated phoresis (galvanisation) with automatically selected frequencies (“Raymedies”), based upon previous performed Eda-measurements.

The cliënt is in a prone position.

- Connect the Zero-electrode (+) with the red cable to the red socket on the front of the Matrix-device, and the dermaroller (-) with the black cable to the black socket. Attach the Zero-electrode to the client’s wrist with the Velcron strap and a moisturized tissue pad.
- Turn the switch in the “ON” position. Make sure that the rod-antenna has been connected to the back of the device. In case of an insufficient wireless connection, an error message will be shown, which will disappear after having performed the proper procedure. (see picture). The current amplitude can be adjusted by moving the cursor along the vertical column at the right side of the screen. It should be adjusted just below the sensitive level.

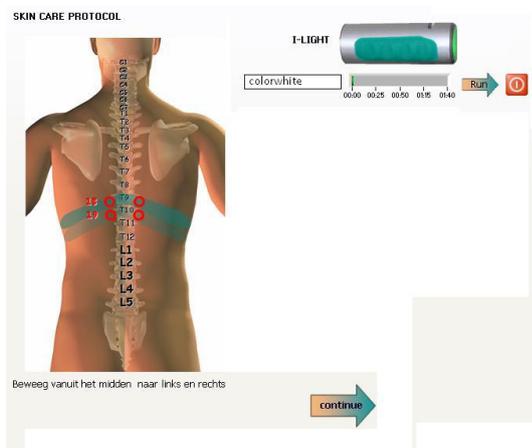

- Apply the Aloe-Restorate-mixture to the indicated skin areas.
- Treat the indicated points with the i-LIGHT, at a distance of approx. 10 cm. Move the **i-LIGHT** from the spinal centre of the indicated dermatome towards left and right
- Klick the “RUN” arrow next to the upper indicated Raymedy. Now move with the **dermaroller** from the spinal centre of the indicated dermatome towards left and right.

The treatment time has been preset on more than 1 minute, but you can repeat the procedure for each dermatome, or abort it at any moment.

- By clicking on the “RUN” arrow next to the second indicated Raymedy, that one will be activated. After having finished the whole first step, click on the “CONTINUE”-arrow to enter the next step.




-I-ON:

- Apply aloe vera –restorate mixture
- Connect Dermaroller to black i-Matrix socket
- Connect 0-electrode to red i-Matrix socket
- Adapt current amplitude to a sub-sensitive level
- Activate Raymedies by clicking on the “run” –arrow
- Treat indicated dermal zones with the dermaroller
- Click “continue” arrow to enter the next step

5.1.2 REGENERATION PROGRAM 1, STEP 2


Now you are ready for the second stage of the regeneration program: pulsating vacuum massage. Remove the remaining mixture carefully with a warm moisturized towel and prepare the back of your client with almond oil, mixed with the coded essential oil complex as indicated on your screen. In this particular example, start with 2 vacuum cups in the neck, and activate the i-VAC by clicking the “RUN”-arrow right below. Follow the on-screen instructions. When you are ready with the second stage, click the “CONTINUE”- arrow right below the screen.

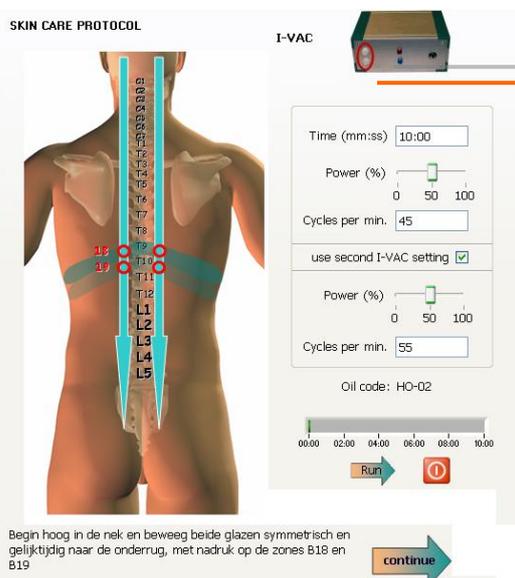

- Apply almond oil on the back, mixed with the coded essential oil complex
- Start the vacuum cupping by clicking the small “RUN”- arrow
- Move both big vacuum cups symmetrically and simultaneously along the spine, in the indicated direction
- Apply 7-8 suction-cycles to the indicated points
- Continue the program by clicking the “CONTINUE”-arrow
- Remove the remaining oil carefully with a warm moistured towel

5.1.3 REGENERATION PROGRAM 1, STEP 3

Now, you are in the 3rd stage of the regeneration program: treatment of the indicated zones with the i-LIGHT. Activate the Raymedies by clicking the “RUN”-arrow. Click the “CONTINUE”-arrow when you are finished.

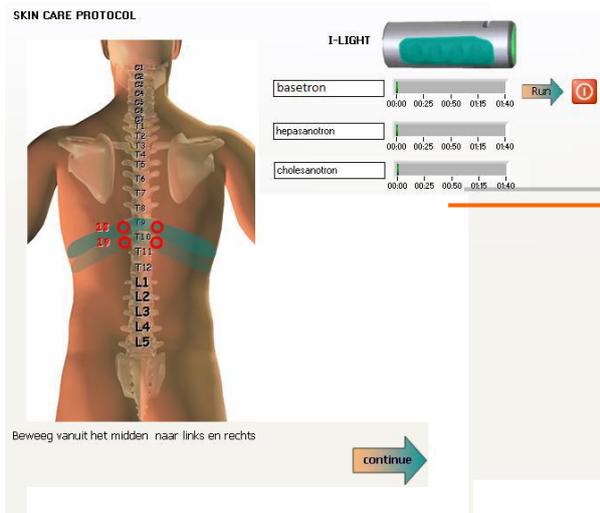

- Treat the indicated points with the i-LIGHT, at a 10 cm distance
- Start the treatment by clicking the “RUN”- arrow next to the indicated Raymedies
- Continue the program by clicking the arrow right below the screen

Doing that, the program asks you to do another EDA measurement. Again, click the big arrow.




Help		
Test 1 meridaan		
Middelen instellen		
5109	Lo 11	3540
4937	Di 1	3498
4144	C 9	3926
3634	3E 1	4588
3383	H 9	4869
3419	Du 1	4873
4889	MP 1	4941
4726	Le 1	5086
4844	M 45	5852
4836	G 44	6827
4912	N 1	7203
4928	B 67	6319

5.1.4 ELIMINATION, STEP 4

Now, you have to click the blinking arrow in the upper screen part, to enter the 4th stage of the regeneration program: Elimination. Your client is in supine position, with uncovered abdomen. Use the proper oil combination, and activate the i-VAC by clicking the small “RUN”- arrow.

Start with a small cup:

- Start with a small cup in the clavicle groove (acupuncture point St11): 7-8 suction cycles
- Between the big toe and the second toe (acupuncture point Liv3): 7-8 suction cycles
- Continue with a big cup at the inner knee side (acupuncture point Liv8): 7-8 suction cycles
- Thereafter, move the big cup from the outer side of the hip region to the inner side
- Continue applying two big cups to the left and right abdominal area, and move according to the indicated arrows to the centre, then from the left and right side to the upper abdomen, then again from both abdominal sides to the pubic area
- Finally, follow the indicated arrow direction along the Conception-vessel
- Remove the oil remains carefully with a warm moisturized towel

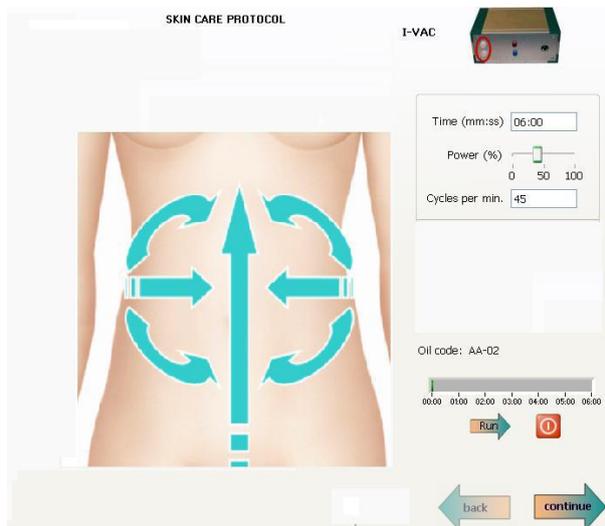

ELIMINATION, STEP 4:

- Client in supine position
- Use the proper oil combination (in this case AA-3)
- Apply enough oil to the treatment zones
- Click the “run”-arrow to activate the i-VAC
- First treat with a small cup the points Liv3 and Liv8
- Continue with both big vacuum cups as indicated
- Click the “continue”- arrow to move on

Again the program asks you to perform an EDA measurement, After having done that, clicking the “continue”- arrow will lead you to the 5th and last stage of this program.

Please do 1 EDA measurement for the i-health skin analysis.




continue

Help		
Test 1 meridiaan		Middelen instellen
5109	Lo 11	3540
4937	Di 1	3498
4144	C 9	3926
3634	3E 1	4588
3383	H 9	4869
3419	Du 1	4873
4889	MP 1	4941
4726	Le 1	5086
4844	M 45	5852
4836	G 44	6827
4912	N 1	7203
4928	B 67	6319

5.1.5 CONSOLIDATION, STEP 5

In order to proceed to the consolidation stage, connect the red Beamer plug to the i-Matrix device, and apply the red beamer to the indicated point as shown in the picture. Just activate the proper Raymedy by clicking the “run”-arrow next to the indicated Raymedy.

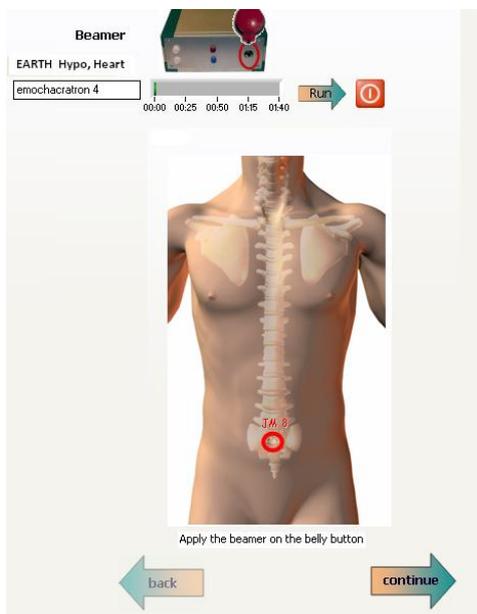

CONSOLIDATION:

- Client in supine position
- Connect the red beamer to the i-MATRIX, and apply the beamer to the indicated area
- Click the “run”-arrow to activate the proper Raymedy
- Click the “continue”-arrow to move on

In case your client feels very cold after this treatment, it is recommended to finish the abdominal treatment with a local 15 minute TDP-heat application. Clicking the “continue”-arrow will inform you to have finished this program, with the text:

Protocoll is finished.

5.2 SKIN CARE II: FACIAL REGENERATION –DETOX AND REVITALISATION OF FACIAL ZONES




SKIN CARE PROTOCOL

First, apply a mixture of Aloe vera gel and Restorate (ratio: 2 table spoons : 1 level tea spoon) to the whole neck.

We discovered that radiation with white light, prior to i-ON applications creates an optimal alkalizing and remineralization skin effect after the application of the above mentioned mixture. That's why an extra i-LIGHT application with white light has been programmed in almost all treatment protocols. So just follow the indications on screen.


5.2.1 SKIN CARE II – FACIAL REGENERATION, STEP 1A: I-ON TREATMENT.

Thereafter, the neck zones will be treated, with the i-ON, i-VAC and i-LIGHT.

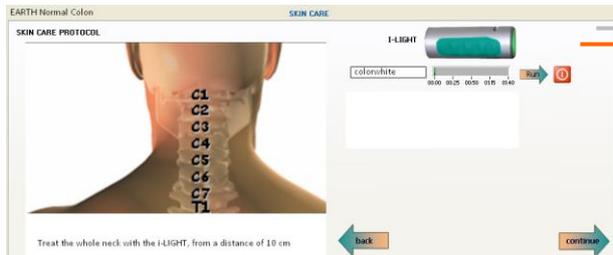

i- i-LIGHT PREPARATION PRECEDING I-ON TREATMENT:


- Client in prone position
- Apply the aloe-restore mixture to the neck area
- Beam the i-LIGHT to the neck, at a 10 cm distance
- Click “run” to activate the i-LIGHT
- Click the “Continue”-arrow to move on

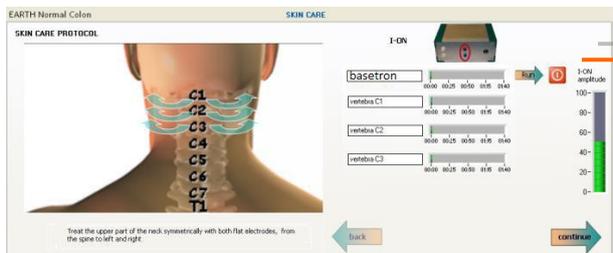

i-ON SKIN CARE II, STEP 1A i-ON NECK TREATMENT

- Client in prone position; adjust the proper current amplitude
- Connect Dermaroller to the black i-Matrix socket
- Connect 0-electrode to the red socket and the wrist joint
- Click the “run”-arrow to activate “basatron” and treat the whole neck area with the Dermaroller, then push the red button to interrupt
- Connect the black cable to the second black cable and click the “run”-arrow again
- treat the upper neck part symmetrically with the 2 flat rod electrodes from the spine centre to left and right with the proper raymedies
- Remove the aloe-restore remains with a warm towel
- Click the “Continue”-arrow to move on


5.2.1 SKIN CARE II – FACIAL REGENERATION, STEP 1B: I-VAC TREATMENT.

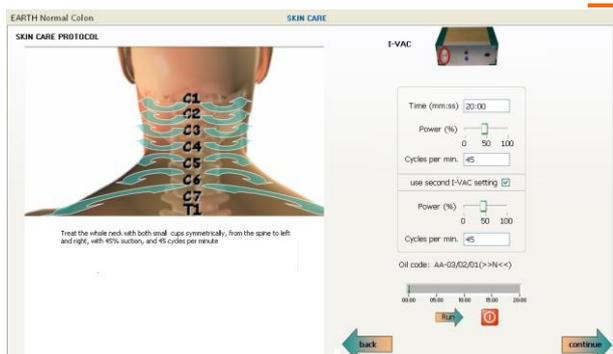

i-VAC SKIN CARE II, STEP 1B:


- Client in prone position
- Apply the proper oil combination to the treatment zone (in this case: Earth-normal-AA-02)
- Click “run” to activate the i-VAC
- Use the small vacuum cups according to the instructions
- Remove the remaining oil with a warm moisturized towel
- Click “Continue” to move on

5.2.1 SKIN CARE II – FACIAL REGENERATION, STEP 1C: I-LIGHT TREATMENT.

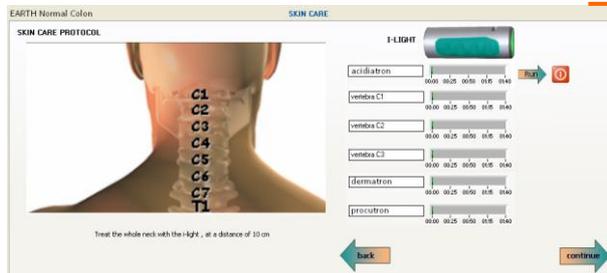

i-LIGHT SKIN CARE II, STEP 1C: i-LIGHT TREATMENT

- Client in prone position
- Beam the i-LIGHT to the neck, at a 10 cm distance
- Click "run" to activate the i-LIGHT
- Click the "Continue"-arrow to move on

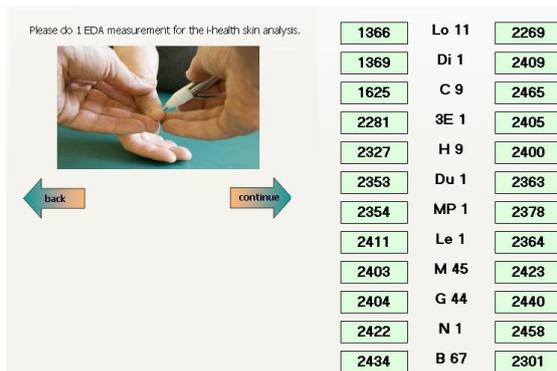


NEW EDA MEASUREMENT


- A next EDA measurement is necessary, preceding the facial revitalization
- Follow the instructions on screen

5.2.2 SKIN CARE II, FACIAL REGENERATION, STEP 2A: FACIAL TREATMENT WITH I-ON .




Clean the facial skin. First, apply a mixture of Aloe vera gel and Restorate. Then, radiate the whole face with the i-LIGHT, color white. Adjust the i-ON amplitude to a subsensitive level (normally between 70 and 80, if the zero-electrode is well moisturized), and activate the Raymedy by clicking the "run"-arrow. Thereafter, the whole face will be treated with the dermaroller, with the Raymedies Cicatron and Basetron. .

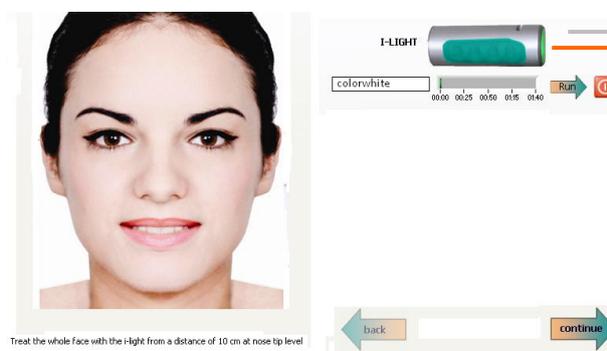

i-LIGHT PREPARATION PRECEDING i-ON TREATMENT:
Radiate the whole face with the color white, to facilitate the absorption of the mixture into the skin

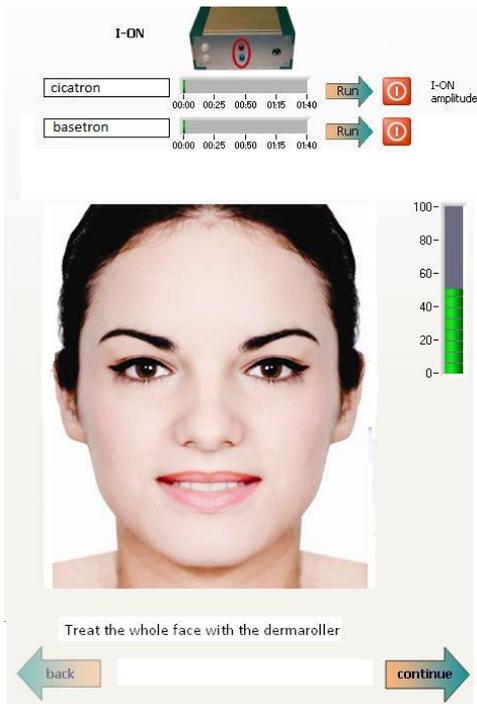


i-ON SKIN CARE II, STEP 2A. According to the weakest meridian in the previous EDA-measurement, 3 specific facial zones will be treated subsequently with the 2 rod-electrodes .

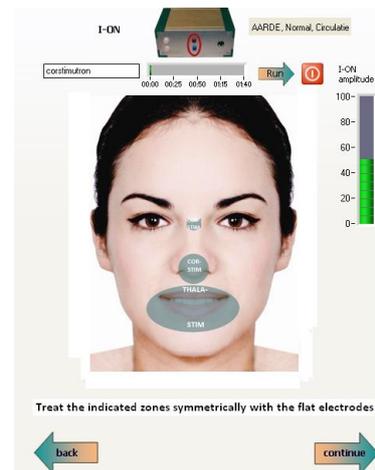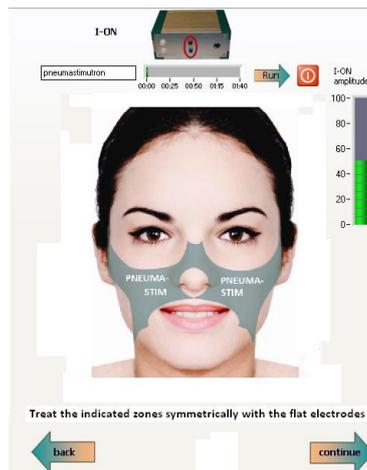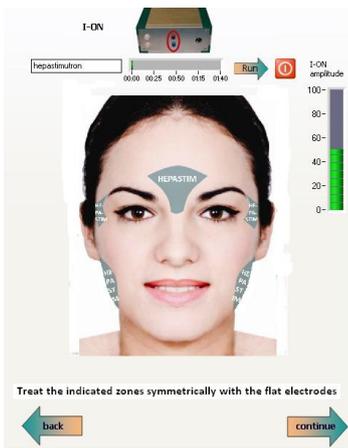


5.2.2 SKIN CARE II - FACIAL REGENERATION, STEP 2B. FACIAL CUPPING

Treatment with the i-VAC in 2 steps: lymph drainage and connective tissue massage. According to suction power, pulsation and direction of movement, the i-VAC treatment either will have a draining effect on the lymphatic system, or a detoxifying and regenerating effect on the connective tissues.


- Remove the remaining aloe-mixture, and apply to the face a mixture of almond oil and the coded element complex as indicated on screen. Then, use the smallest cups as follows:
- Lymph drainage
 1. In the clavicular groove (acupuncture point St11): 7-8 suction cycles
 2. From the center of the lower lip across the lower edge of the chin
 3. With both cups from the lower lip across the lower edge of the chin
 4. From the nasolabial wrinkle across the lower edge of the chin (see picture)
 5. From the cheeks across the lower edge of the chin (see picture)
 6. From the middle lower edge of the chin sideward to a depression below the ear lobes (acupuncture point TH 17)
 7. From TH17 to the clavicular groove (St11): 7-8 suction cycles
 8. From the inner eye corner to the outer eye corner (Tai Yang)
 9. From Yin Tang (between the eye brows) to the hair border
 10. From the forehead center across the temporal area to Tai Yang: 3-4 suction cycles
 11. From Tai Yang to the depression below the ear lobe (TH17): 3-4 suction cycles
 12. From there to the clavicular groove (St11) 7-8 suction cycles
- Connective tissue massage, stage 1 (55 cycles)
 1. From the centre below the lips in one upward movement (see picture)
 2. From the cheek area in one upward movement
 3. From the centre of the forehead sideward
- Connective tissue massage, stage 2 (550 cycles): Change the cycle range into 550 and use the flat cup
 1. From the centre below the lips in one upward movement
 2. From the cheek area in one upward movement
 3. From the forehead centre sideward
- Remove carefully the oil remains with a moisturized warm towel

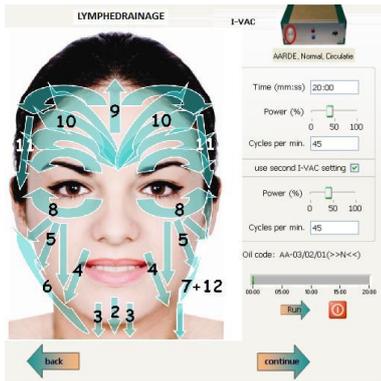

i-VAC: According to the vacuum power, pulsation and moving direction, the i-VAC treatment will have a draining effect on the lymphatic system or a detoxifying and regenerating effect on the connective tissue

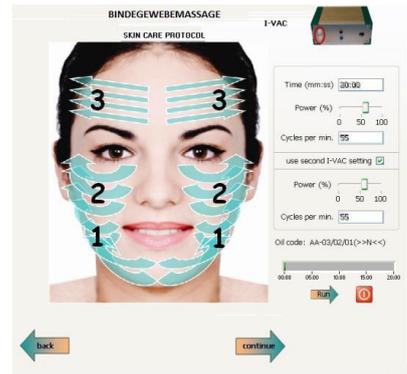

5.2.3 SKIN CARE II - FACIAL REGENERATION, STEP 2C. FACIAL TREATMENT WITH THE I-LIGHT.

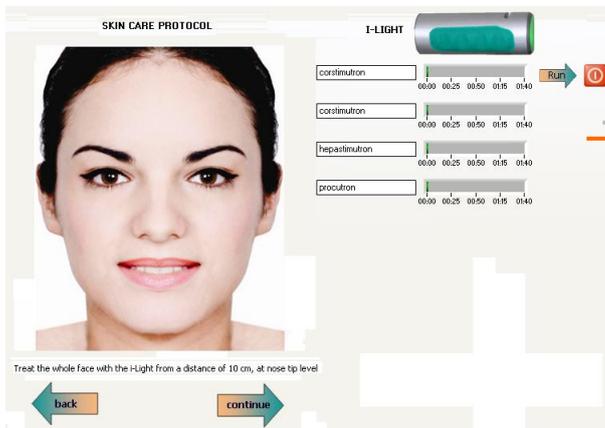

i-LIGHT SKIN CARE II, STEP 2C: the facial skin receives similar meridian regulating Raymedies as in step 2a, but now as color signals with the i-LIGHT, with a powerful skin vitalizing Raymedy at the end

Beam the i-LIGHT at nose level on a distance of 10 cm from the face, and click "run".


A final EDA measurement is necessary to define the proper Raymedy for the consolidation stage.

Please do 1. EDA measurement for the i-Health skin analysis.

1366	Lo 11	2269
1369	Di 1	2409
1625	C 9	2465
2281	3E 1	2405
2327	H 9	2400
2353	Du 1	2363
2354	MP 1	2378
2411	Le 1	2364
2403	M 45	2423
2404	G 44	2440
2422	N 1	2458
2434	B 67	2301

5.2.4 SKIN CARE II – FACIAL REGENERATION, STEP 3: CONSOLIDATION

In order to perform the consolidation stage as the last step of this program, connect the red Beamer to the i-Matrix device, and apply the beamer to the indicated area. Now activate the proper Raymedy by clicking the “run”-arrow, next to the mentioned Raymedy.

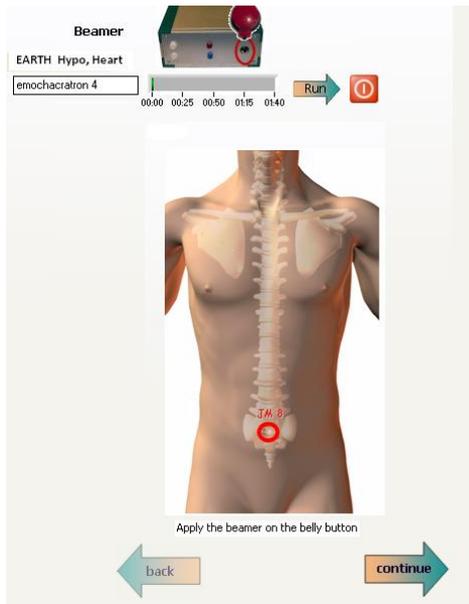


BEAMER SKIN CARE II, STEP 3: CONSOLIDATION:

- Client in supine position
- Connect the red beamer to i-MATRIX, and apply the Beamer on the indicated area
- Click the “run”-arrow to activate the indicated Raymedy
- Click the “continue”-arrow to move on

By clicking the “continue”-arrow, you will be notified you just finished this program.

Procoll is finished.

5.3 REJUVENATION PROGRAM

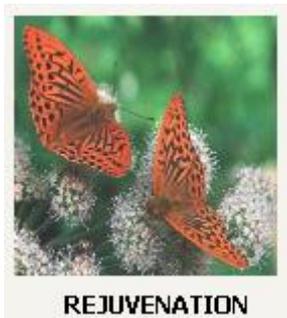


QUICKVIEW REJUVENATION PROGRAM (ANTI-AGE)

1. 8 Min facial radiation with Infrared light (TDP-lamp)
2. 3 EDA measurements
3. Application with Aloe+Restorate mixture in the neck
4. I-LIGHT with white light
5. I-ON according to protocol with Aloe+Restorate, with the first Raymedy (basetron) the whole neck is treated with the Dermalroller
6. I-ON (see picture): the upper 3 vertebrae + dermatomes with the indicated raymedies and both flat rod electrodes
7. I-VAC according to protocol with almond oil +5 Elements complex
8. I-LIGHT according to protocol
9. Facial mask with Aloe+Restorate
10. I-LIGHT with white light
11. i-ON with the dermaroller with Cicatron and Basetron
12. Remove the remains of Aloe+Restorate, continue I-ON protocol with Aloe + Q10 + Beauty Line 12h active serum

13. I-VAC according to protocol with almond oil + 5 elements Complex
14. I-LIGHT according to protocol
15. EDA measurement
16. Beamer Emochacraton


Start the Rejuvenation Program.

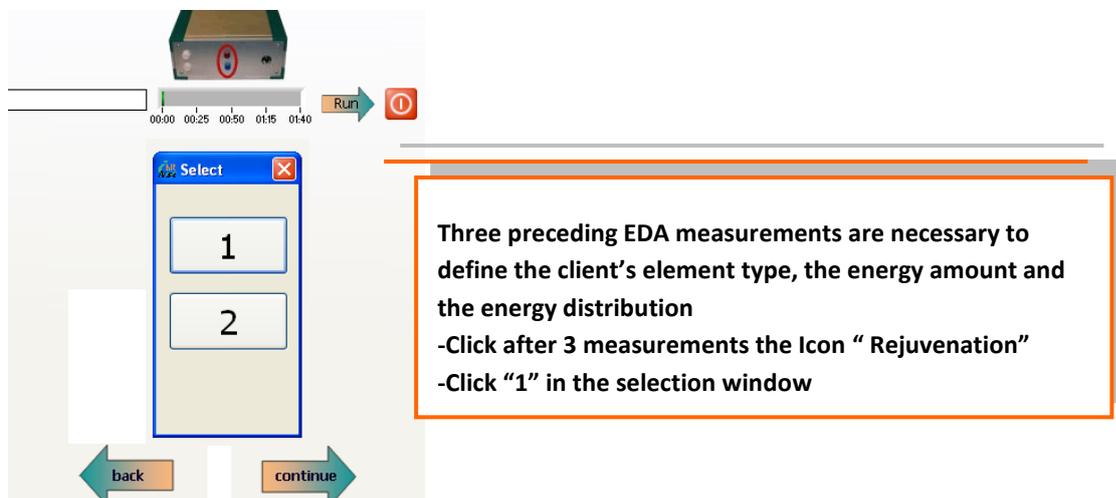

As mentioned before, the i-ON program will start with facial radiation with the color white with the i-LIGHT.

5.3.1 REJUVENATION OF THE NECK WITH THE I-ON


Prepare a mixture of Aloe+restorate, and apply that mixture to the whole neck

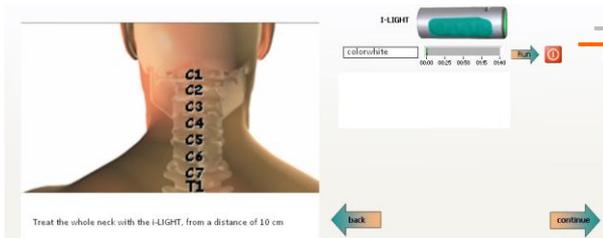

i- i-LIGHT PREPARATION PRECEDING I-ON TREATMENT:

- Client in prone position
- Apply the aloe+restorate mixture to the treatment zone
- Beam the i-LIGHT to the neck, at a 10 cm distance


After that, the next screen will appear:

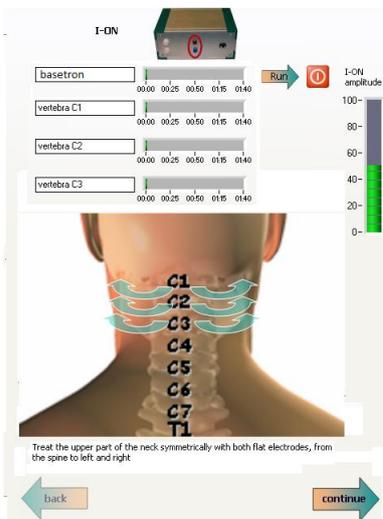

NECK REJUVENATION WITH i-ON:

- Client in prone position
- Attach the 0 (red)-electrode to the client's wrist
- Adjust the proper current amplitude
- Click the "run"-arrow to activate the first Raymedy, and treat the whole neck with the Dermaroller. Then, click "stop".
- After that, connect the 2nd black cable to the 1st one, connect the 2 flat rod electrodes to both ones, activate the other Raymedies and treat the corresponding vertebrae with them
- Remove the aloe-restorate remains
- Click the "continue"-arrow to move on


5.3.2 REJUVENATION OF THE NECK WITH THE I-VAC

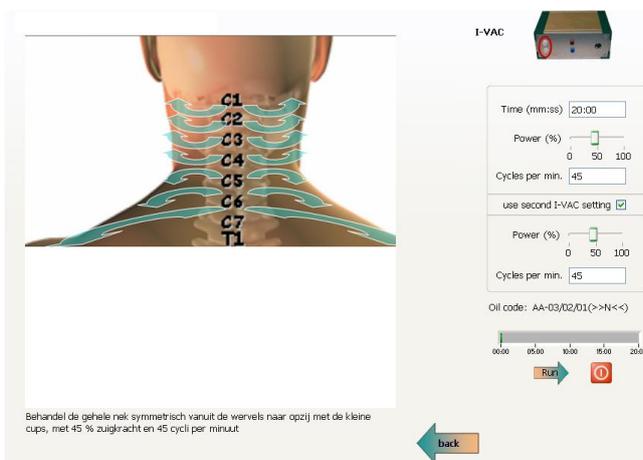

NECK REJUVENATION WITH i-VAC:

- Client in prone position
- Apply almond oil to the treatment zone, mixed with the proper element complex as indicated on screen
- Click "run" to activate the i-VAC device
- Use the small vacuum-cups according to instructions
- Remove the oil remains
- Click the "continue"-arrow when you are ready with this step

5.3.3 REJUVENATION OF THE NECK WITH THE I-LIGHT

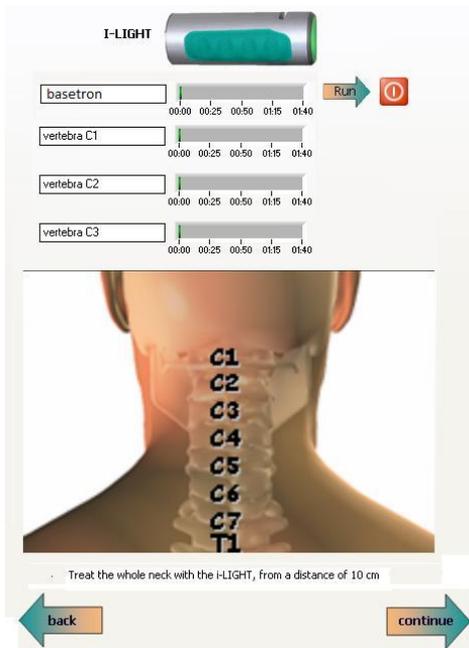


NECK REJUVENATION WITH i-LIGHT:

- Client in prone position
- Beam the i-LIGHT to the neck, at a 10 cm distance
- Click “run” to activate the i-LIGHT
- Click “continue” to move on when finished with this procedure


5.3.4 FACIAL REJUVENATION WITH THE I-ON

Clean the face with rose water. Then apply a facial mask of Aloe-Restorate and radiate the face with white light from the i-LIGHT. Ask the client to keep the eyes closed during this procedure.

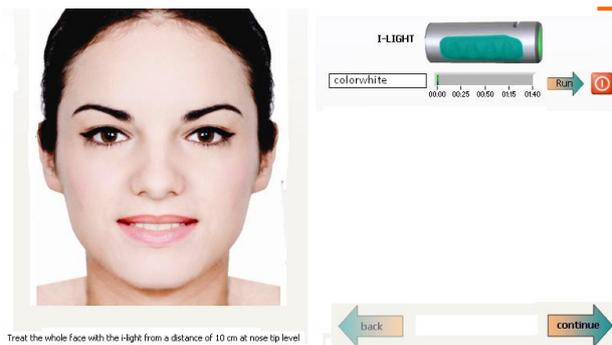

i-LIGHT PREPARATION PRECEDING I-ON TREATMENT:

- Client in supine position, with eyes closed
- Beam the i-LIGHT to the face, at a 10 cm distance
- Click “run” to activate the i-LIGHT
- Click the “Continue”-arrow to move on

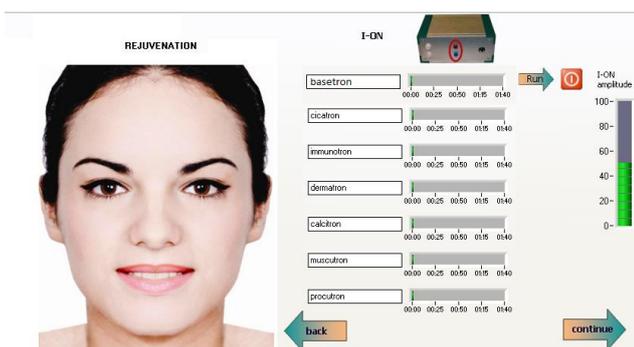


FACIAL REJUVENATION WITH i-ON:


- Client in supine position
- Attach the (red) 0-electrode to the wrist
- Adjust the proper current amplitude
- Click the “run”-arrow to activate the first 2 Raymedies
- Treat the whole face with the dermaroller
- Remove the remains of Aloe+Restorate, and apply a new mask with Aloe+Q10+Beauty line 12h Serum (1TS:7dr:6 sprays)
- Continue the protocol
- Click “continue” to move on when finished

5.3.5 FACIAL REJUVENATION WITH THE I-VAC IN 2 STAGES: LYMPH DRAINAGE AND CONNECTIVE TISSUE MASSAGE.

Remove the remaining contact-gel, and prepare a mixture of almond oil and the element complex as indicated on screen

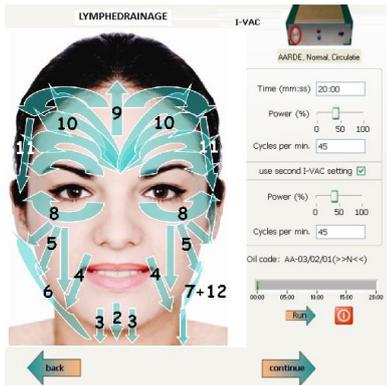

i-VAC: According to the vacuum power, pulsation and moving direction, the i-VAC treatment will have a draining effect on the lymphatic system or a detoxifying and regenerating effect on the connective tissue

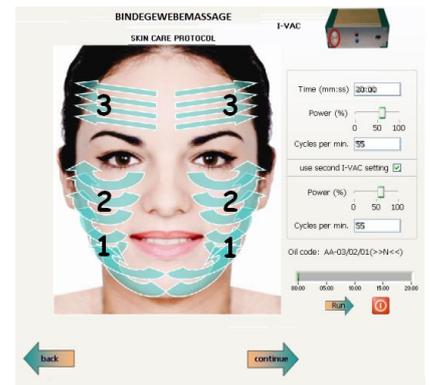


- **Lymph drainage**

1. In the clavicular groove (acupuncture point St11): 7-8 suction cycles
2. From the center of the lower lip across the lower edge of the chin
3. With both cups from the lower lip across the lower edge of the chin
4. From the nasolabial wrinkle across the lower edge of the chin (see picture)
5. From the cheeks across the lower edge of the chin (see picture)
6. From the middle lower edge of the chin sideward to a depression below the ear lobes (acupuncture point TH 17)
7. From 3H17 to the clavicular groove (St11): 7-8 suction cycles
8. From the inner eye corner to the outer eye corner (Tai Yang)
9. From Yin Tang (between the eye brows) to the hair border
10. From the forehead center across the temporal area to Tae Yang: 3-4 suction cycles
11. From Tae Yang to the depression below the ear lobe (TH17): 3-4 suction cycles
12. From there to the clavicular groove (St11) 7-8 suction cycles

- **Connective tissue massage, stage 1 (55 cycles)**


1. From the centre below the lips in one upward movement (see picture)
 2. From the cheek area in one upward movement
 3. From the centre of the forehead sideward
- Connective tissue massage, stage 2 (550 cycles): Change the cycle range into 550 and use the flat cup
 1. From the centre below the lips in one upward movement
 2. From the cheek area in one upward movement
 3. From the forehead centre sideward
 - Remove carefully the oil remains with a moisturized warm towel

5.3.6 FACIAL REJUVENATION WITH THE I-LIGHT

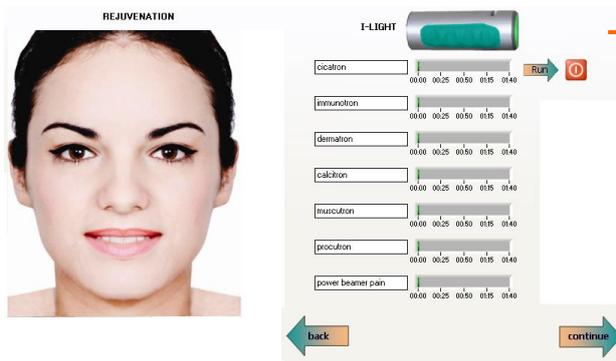

FACIAL REJUVENATION WITH i-LIGHT:


- Client in supine position, with closed eyes
- Beam the i-LIGHT to the face at nose tip level, at a 10 cm distance
- activate the Raymedies by clicking the "Run"-arrow
- Click "continue" to move on when finished

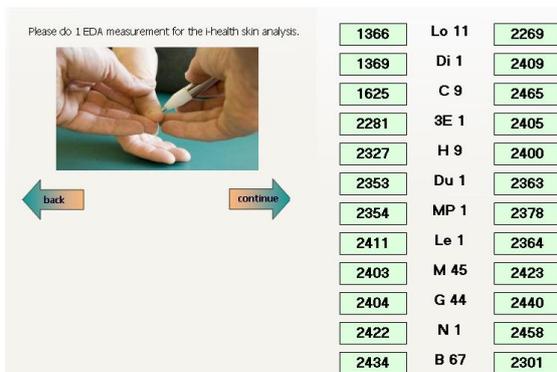

NEW EDA MEASUREMENT

- A next EDA measurement is necessary, preceding the facial revitalization
- Follow the instructions on screen

5.3.7 FINAL REJUVENATION STAGE - CONSOLIDATION WITH THE BEAMER

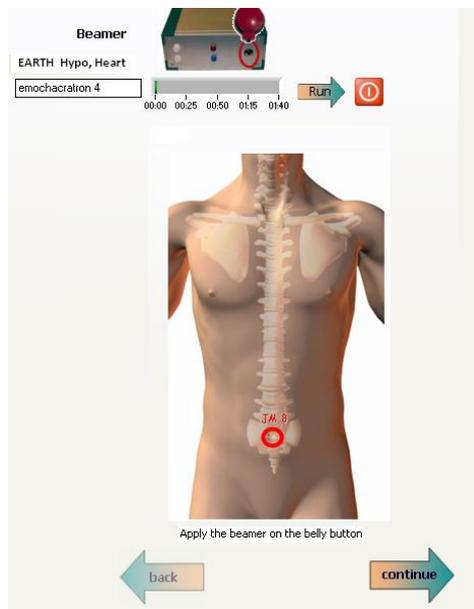

FINAL REJUVENATION STAGE: CONSOLIDATION

- Client in supine position
- Due to the actual energy excess in the Earth Element (in this example) , automatically the program has selected the Raymedy Emochacatron 5: discharge of energy excess to Metal
- Apply the red beamer to the navel, and activate the Raymedy by clicking the “run”-arrow

This program will be finished after having clicked the “continue”-arrow:

Protocoll is finished.

5.4 ANTI-WRINKLE PROGRAM



ANTI-WRINKLE


QUICKVIEW ANTI-WRINKLE PROGRAM

Together with your client, select 1 to approx. 2 problematic wrinkle zones to treat in one session

1. 8 Min facial radiation with Infrared light (TDP-lamp)
2. 3 EDA measurements
3. Application with Aloe+Restorate in the neck
4. I-LIGHT with white light
5. I-ON according to protocol with Aloe+Restorate, with the first Raymedy (Basetron) the whole neck is treated with the dermaroller
6. I-ON (see picture): the upper 3 vertebrae +dermatomes with the related Raymedies and both flat rod electrodes
7. i-VAC according to protocol with almond oil +5 Elements complex
8. I-LIGHT according to protocol
9. Facial mask with Aloe+Restorate
10. I-LIGHT with white light
11. i-ON with the dermaroller with Cicatron and Basetron
12. Remove the remains of Aloe+Restorate, continue I-ON protocol with Aloe+Q10 +Beauty Line 12h Serum and both spherical rod electrodes
13. I-VAC according to protocol with almond oil + 5 elements CPL
14. I_LIGHT according to protocol
15. EDA measurement
16. Emochakraton with beamer


5.4.1 PREPARATORY ANTI-WRINKLE NECK TREATMENT WITH THE I-ON

Start with application of Aloe+Restorate in the neck, followed by I-LIGHT with white light. Thereafter you can continue with the i-ON procedure

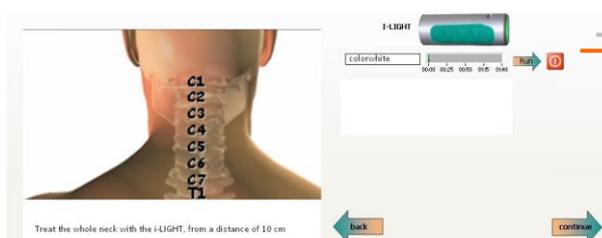

i- i-LIGHT PREPARATION PRECEDING I-ON TREATMENT:


- Client in prone position
- Apply aloe+restorate to the treatment zone
- Beam the i-LIGHT to the neck, at a 10 cm distance
- Click "run" to activate the i-LIGHT

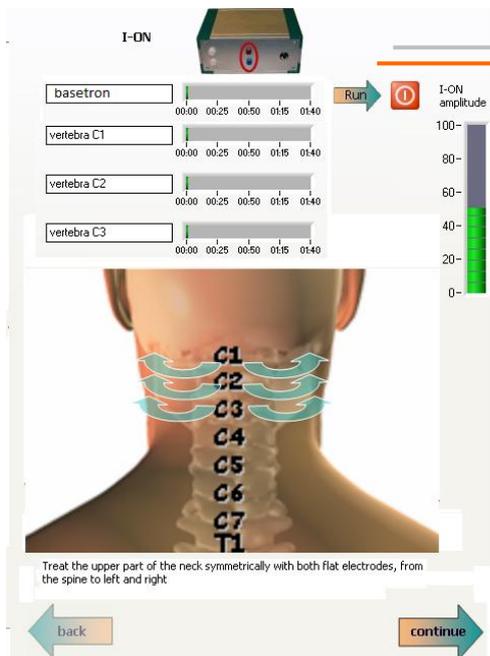

Anti-wrinkle treatment with i-ON:

- Client in prone position
- Attach the **(red) 0**-electrode to the client's wrist
- Adjust the proper current amplitude
- Click the "run"-arrow to activate the first Raymedy, and treat the whole neck with the Dermalroller
- After that, click "stop", connect the 2nd black cable to the 1st one, connect both ones to the flat rod electrodes, activate the other Raymedies and treat the corresponding vertebrae symmetrically as indicated
- Remove the Aloe-Restorate-mixture
- Click the "continue"-arrow to move on


5.4.2 ANTI-WRINKLE NECK TREATMENT WITH THE I-VAC

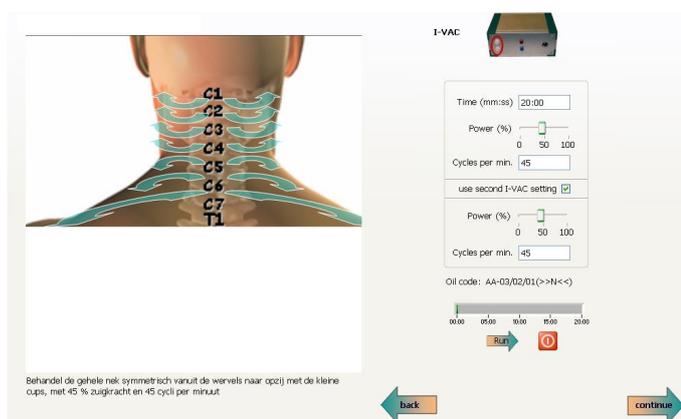

Anti-wrinkle treatment with i-VAC:

- Client in prone position
- Apply almond oil to the treatment zone, mixed with the proper element complex as indicated on screen
- Click "run" to activate the i-VAC device
- Use the small vacuum-cups according to instructions
- Remove the oil remains carefully
- Click the "continue"-arrow when you are ready with this step

5.4.3 ANTI-WRINKLE NECK TREATMENT WITH THE I-LIGHT

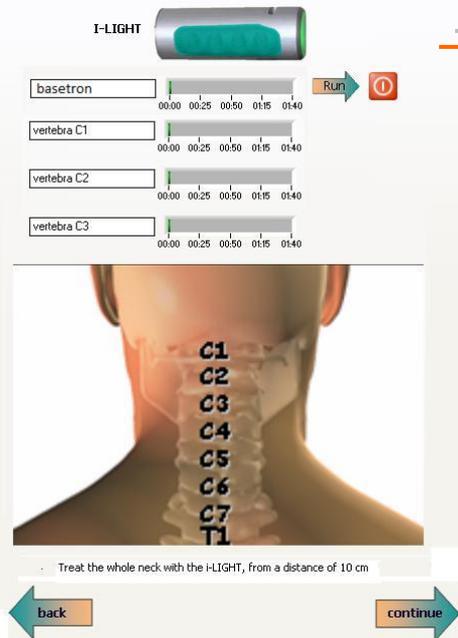


Anti-wrinkle treatment with i-LIGHT:

- Client in supine position
- Beam the i-LIGHT to the neck, at a 10 cm distance
- Click “run” to activate the i-LIGHT
- Click “continue” to move on when finished with this procedure

5.4.4 TREATMENT OF THE MOST COMMON WRINKLES WITH THE I-ON

Within the usual consultation time it is not possible to treat all wrinkles thoroughly in one consultation. So discuss the most problematic wrinkles with your client, give those wrinkles treatment priority and follow the treatment instructions on screen. Prepare two mixtures: one mixture of Aloe+Restorate, another one of Aloe+Q10+Rebuild25. Use extra Rebuild 25 directly on the wrinkles to be treated.


Clean the face with rose water. Then apply a facial mask of Aloe-Restorate and radiate the face with white light from the i-LIGHT. Ask the client to keep the eyes closed during this procedure.

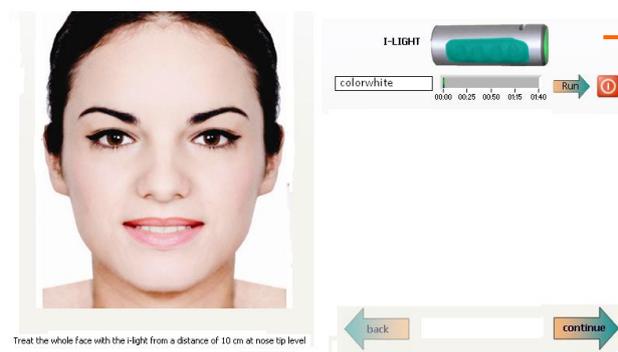

i-LIGHT PREPARATION PRECEDING I-ON TREATMENT:

- Client in supine position, with eyes closed
- Beam the i-LIGHT to the face, at a 10 cm distance
- Click “run” to activate the i-LIGHT
- Click the “Continue”-arrow to move on

ANTI-WRINKLE

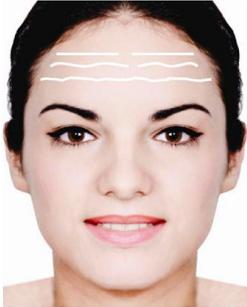

I-ON



calciton	00:00	00:25	00:50	01:15	01:40
calciton	00:00	00:25	00:50	01:15	01:40
dematron	00:00	00:25	00:50	01:15	01:40
immunotron	00:00	00:25	00:50	01:15	01:40
renastimulatron	00:00	00:25	00:50	01:15	01:40
muscutron	00:00	00:25	00:50	01:15	01:40
procutron	00:00	00:25	00:50	01:15	01:40

I-ON amplitude: 0, 20, 40, 60, 80, 100

The demaroller should be connected to the black socket. Treat de whole face with the demaroller during the first 2 minutes. Thereafter, treat the forehead wrinkles with the next six treatment signals with 1 flat electrode. Finish this treatment stage with the demaroller for the whole face, during the last 2 minutes.

[back](#) [continue](#)

ANTI-WRINKLE



I-ON



calciton	00:00	00:25	00:50	01:15	01:40
calciton	00:00	00:25	00:50	01:15	01:40
dematron	00:00	00:25	00:50	01:15	01:40
immunotron	00:00	00:25	00:50	01:15	01:40
hepastimulatron	00:00	00:25	00:50	01:15	01:40
muscutron	00:00	00:25	00:50	01:15	01:40
procutron	00:00	00:25	00:50	01:15	01:40

I-ON amplitude: 0, 20, 40, 60, 80, 100

Treat de whole face with the demaroller during the first 2 minutes, connected to the black socket. Thereafter the frown wrinkles with 1 flat electrode. Finish this treatment stage with the demaroller for the whole face, during the last 2 minutes.

[back](#) [continue](#)

ANTI-WRINKLE



I-ON



calciton	00:00	00:25	00:50	01:15	01:40
calciton	00:00	00:25	00:50	01:15	01:40
dematron	00:00	00:25	00:50	01:15	01:40
immunotron	00:00	00:25	00:50	01:15	01:40
constimulatron	00:00	00:25	00:50	01:15	01:40
muscutron	00:00	00:25	00:50	01:15	01:40
procutron	00:00	00:25	00:50	01:15	01:40

I-ON amplitude: 0, 20, 40, 60, 80, 100

The demaroller should be connected to the black socket. Treat de whole face with the demaroller during the first 2 minutes. Thereafter the upper nose wrinkles with 1 flat electrode. Finish this treatment stage with the demaroller for the whole face, during the last 2 minutes.

[back](#) [continue](#)

ANTI-WRINKLE



I-ON



calciton	00:00	00:25	00:50	01:15	01:40
calciton	00:00	00:25	00:50	01:15	01:40
dematron	00:00	00:25	00:50	01:15	01:40
immunotron	00:00	00:25	00:50	01:15	01:40
hepastimulatron	00:00	00:25	00:50	01:15	01:40
muscutron	00:00	00:25	00:50	01:15	01:40
procutron	00:00	00:25	00:50	01:15	01:40

I-ON amplitude: 0, 20, 40, 60, 80, 100

Treat de whole face with the demaroller, connected to the black socket, during the first 2 minutes. Treat thereafter the crowfeet wrinkles on one side with the next 6 treatment signals with one flat electrode. Then, treat the other side in the same way. Finish this treatment stage with the demaroller for the whole face, during the last 2 minutes.

[back](#) [continue](#)

ANTI-WRINKLE



I-ON



calciton	00:00	00:25	00:50	01:15	01:40
calciton	00:00	00:25	00:50	01:15	01:40
dematron	00:00	00:25	00:50	01:15	01:40
immunotron	00:00	00:25	00:50	01:15	01:40
renastimulatron	00:00	00:25	00:50	01:15	01:40
muscutron	00:00	00:25	00:50	01:15	01:40
procutron	00:00	00:25	00:50	01:15	01:40

I-ON amplitude: 0, 20, 40, 60, 80, 100

The demaroller should be connected to the black socket. Treat the whole face with the demaroller during the first 2 minutes. Thereafter the frontal eye wrinkles with one flat electrode. Finish this treatment stage with the demaroller for the whole face, during the last 2 minutes.

[back](#) [continue](#)

ANTI-WRINKLE



I-ON



calciton	00:00	00:25	00:50	01:15	01:40
calciton	00:00	00:25	00:50	01:15	01:40
dematron	00:00	00:25	00:50	01:15	01:40
immunotron	00:00	00:25	00:50	01:15	01:40
pneumastimulatron	00:00	00:25	00:50	01:15	01:40
muscutron	00:00	00:25	00:50	01:15	01:40
procutron	00:00	00:25	00:50	01:15	01:40

I-ON amplitude: 0, 20, 40, 60, 80, 100

The demaroller should be connected to the black socket. Treat the whole face with the demaroller during the first 2 minutes. Thereafter the nasolabial wrinkles with one flat electrode. Finish this treatment stage with the demaroller for the whole face, during the last 2 minutes.

[back](#) [continue](#)


i-ON treatment Step 1

- Apply Adjust the proper current amplitude. Connect the red cable to your clients wrist, activate the Raymedies Basetron and Cicatron and treat the whole face with the Dermaroller. After that, interrupt by clicking “Stop”

i-ON treatment Step 2

- Remove the Aloe-Restorate remains with a warm moisturized towel
- Apply a warmed mixture of Aloe-Q10-Bauty Line12h Serum (1TS:7dr:6sprays) to the whole face, especially the chosen problematic areas. Be sure you prepare enough Aloe-mixture to finish the job
- Connect the black cable with the 2nd black cable, and connect both ones to the spheroid rod electrodes
- Now click on “run”, to continue the treatment for the chosen facial areas.
- Before you activate the last Raymedy, exchange both rod electrodes for the Dermaroller
- Remove the Aloe-remains before entering the next step in the program

5.4.5 FACIAL LYMPHATIC DRAINAGE AND CONNECTIVE TISSUE MASSAGE WITH THE I-VAC

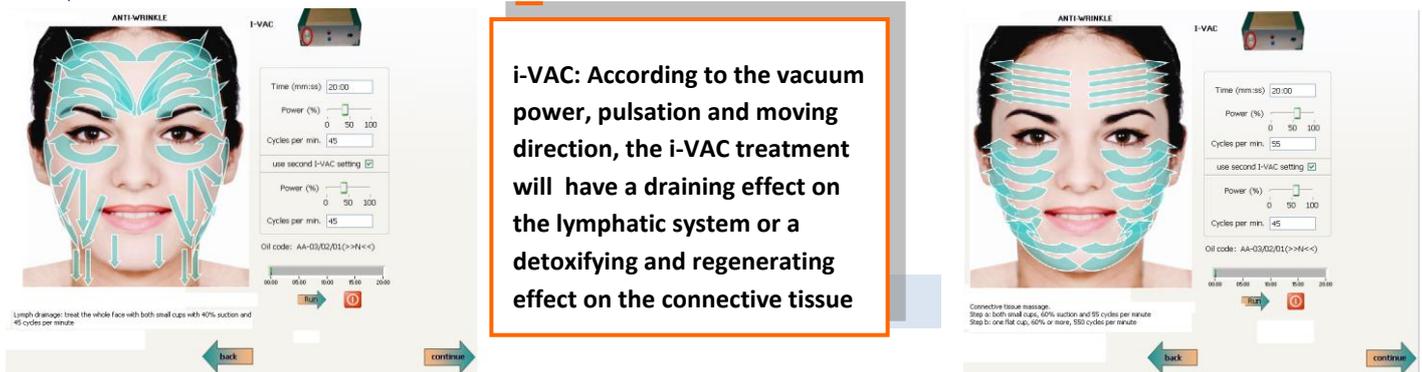

- **Lymph drainage**

1. In the clavicular groove (acupuncture point St11): 7-8 suction cycles
2. From the center of the lower lip across the lower edge of the chin
3. With both cups from the lower lip across the lower edge of the chin
4. From the nasolabial wrinkle across the lower edge of the chin (see picture)
5. From the cheeks across the lower edge of the chin (see picture)
6. From the middle lower edge of the chin sideward to a depression below the ear lobes (acupuncture point TH 17)
7. From 3H17 to the clavicular groove (St11): 7-8 suction cycles
8. From the inner eye corner to the outer eye corner (Tai Yang)
9. From Yin Tang (between the eye brows) to the hair border
10. From the forehead center across the temporal area to Tae Yang: 3-4 suction cycles
11. From Tae Yang to the depression below the ear lobe (TH17): 3-4 suction cycles
12. From there to the clavicular groove (St11) 7-8 suction cycles

- **Connective tissue massage, stage 1 (55 cycles)**


1. From the centre below the lips in one upward movement (see picture)
2. From the cheek area in one upward movement
3. From the centre of the forehead sideward

- **Connective tissue massage, stage 2 (550 cycles): Change the cycle range into 550 and use the flat cup**

1. From the centre below the lips in one upward movement


2. From the cheek area in one upward movement
 3. From the forehead centre sideward
- Remove carefully the oil remains with a moisturized warm towel

5.4.6 FACIAL TREATMENT WITH THE I-LIGHT

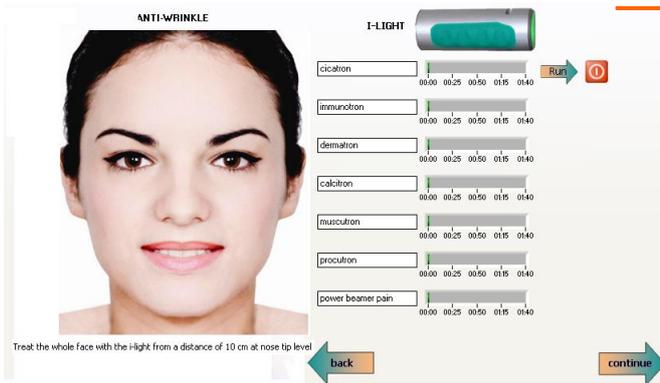

Anti-wrinkle treatment with i-LIGHT:


- Client in supine position, with closed eyes
- Beam the i-LIGHT to the face at nose tip level, at a 10 cm distance
- activate the Raymedies by clicking the "Run"-arrow
- When finished, click "continue" to move on

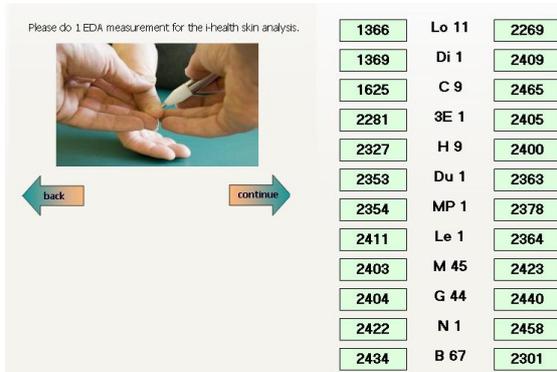

NEW EDA MEASUREMENT

- A next EDA measurement is necessary, preceding the concluding consolidation stage
- Follow the instructions on screen
- When finished, click "continue" to move on

5.4.5 CONSOLIDATION WITH THE BEAMER TO CONCLUDE THE ANTI-WRINKLE PROGRAM

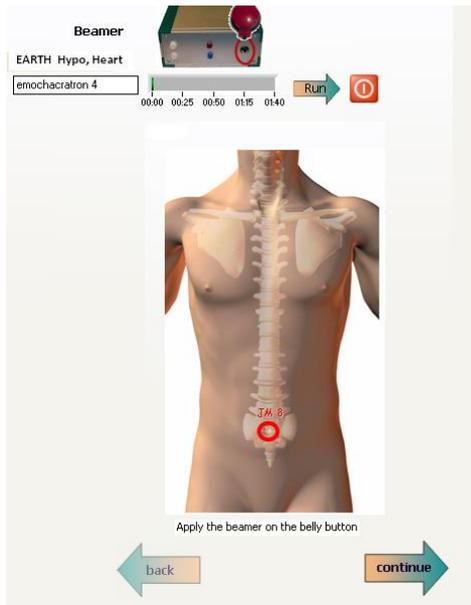

FINAL ANTI-WRINKLE STAGE: CONSOLIDATION

-Client in supine position

- Due to the actual energetic balance in the Earth element in this example, the program selects automatically the Raymedy Eموchacratron 2: stabilizing the personal elemental energy

-Apply the red beamer to the navel and activate the Raymedy by clicking the “run”-arrow

By clicking the “continue”-arrow, the anti-wrinkle program will be finished and closed:

Procoll is finished.

5.5 ACNE PROTOCOL



QUICKVIEW ACNE PROGRAM


1. 10 minutes facial radiation with Infrared light (TDP-lamp)

2. 3 EDA measurements
3. Application with Aloe+Restorate in the neck
4. I-LIGHT with white light
5. I-ON according to protocol with Aloe+Restorate, with the first Raymedy (basetron) the whole neck is treated with the Dermaroller
6. I-ON (see picture): the first 3 Raymedies (and dermatomes) are treated with the related Raymedies and the flat rod electrodes
7. I-VAC according to protocol with almond oil +5 Elements complex
8. I-LIGHT according to protocol

9. Facial mask with Aloe+Restorate
10. I-LIGHT with white light
11. i-ON with the dermaroller with Cicatron and Basetron
12. Remove the remains of Aloe+Restorate, continue I-ON protocol with Aloe+Q10
13. I-VAC according to protocol with almond oil+ 5 Elements complex
14. I-LIGHT according to protocol
15. EDA measurement
16. Emochakraton with beamer


5.5.1 PREPARATORY ACNE TREATMENT OF THE NECK WITH THE I-ON

Start with application of Aloe+Restorate in the neck, followed by I-LIGHT with white light. Thereafter you can continue with the i-ON procedure

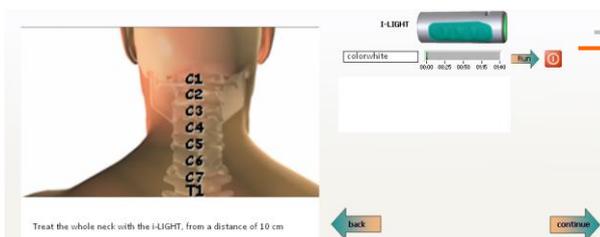

i- i-LIGHT PREPARATION PRECEDING I-ON TREATMENT:


- Client in prone position
- Apply aloe+restorate to the treatment zone
- Beam the i-LIGHT to the neck, at a 10 cm distance
- Click "run" to activate the i-LIGHT

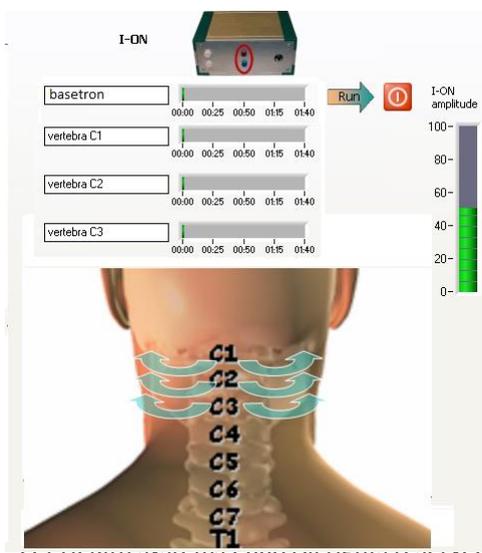

ACNE TREATMENT NECK WITH I-ON:

- Client in prone position
- Attach the 0 (red)-electrode to the client's wrist
- Adjust the proper current amplitude
- Click the "run"-arrow to activate the first Raymedy, and treat the whole neck with the Dermaroller. Then, click "stop".
- After that, connect the 2nd black cable to the 1st one, connect the 2 flat rod electrodes to both ones, continue with the other Raymedies and treat the corresponding vertebrae and their dermatomes
- Remove the aloe-restorate remains
- Click the "continue"-arrow to move on


5.5.2 ACNE TREATMENT OF THE NECK WITH THE I-VAC

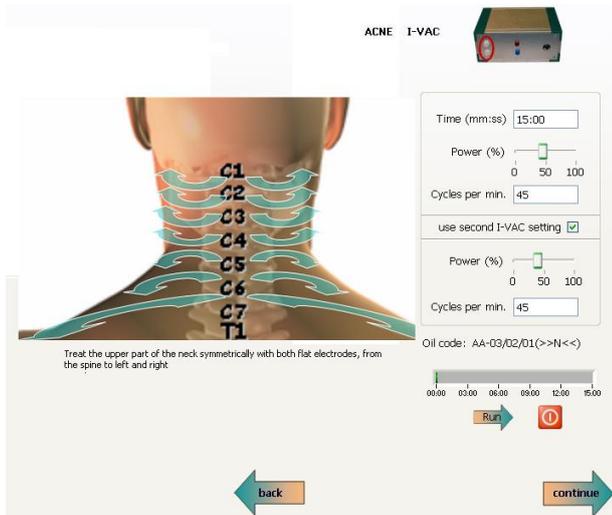

ACNE TREATMENT NECK WITH i-VAC:

- Client in prone position
- Apply almond oil to the treatment zone, mixed with the proper element complex as indicated on screen
- Click "run" to activate the i-VAC device
- Use the small vacuum-cups according to instructions
- Remove the oil remains with a moisturized towel
- Click the "continue"-arrow when you are ready with this step

5.5.3 ACNE TREATMENT OF THE NECK WITH THE I-LIGHT

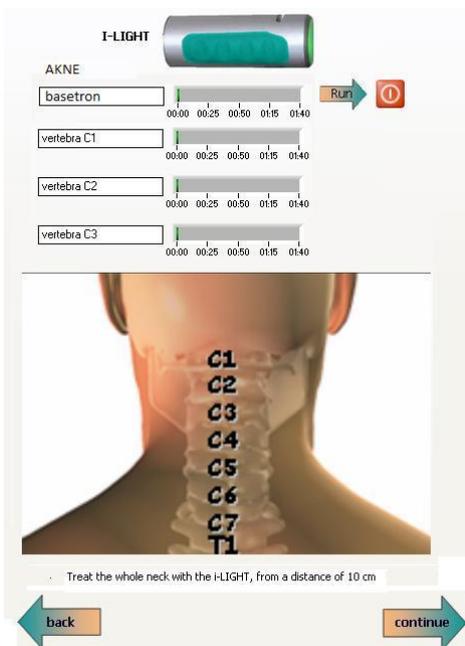


ACNE TREATMENT NECK WITH i-LIGHT:

- Client in prone position
- Beam the i-LIGHT to the neck, at a 10 cm distance
- Click "run" to activate the i-LIGHT
- Click "continue" to move on when finished with this procedure

5.5.4 FACIAL ACNE TREATMENT WITH THE I-ON


Clean the face with rose water. Then apply a facial mask of Aloe-Restorate and radiate the face with white light from the i-LIGHT. Ask the client to keep the eyes closed during this procedure.

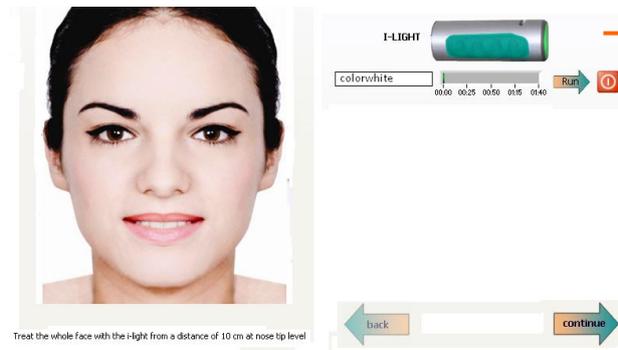

Treat the whole face with the i-light from a distance of 10 cm at nose tip level

i-LIGHT PREPARATION PRECEDING I-ON TREATMENT:

- Client in supine position, with eyes closed
- Beam the i-LIGHT to the face, at a 10 cm distance
- Click “run” to activate the i-LIGHT
- Click the “Continue”-arrow to move on

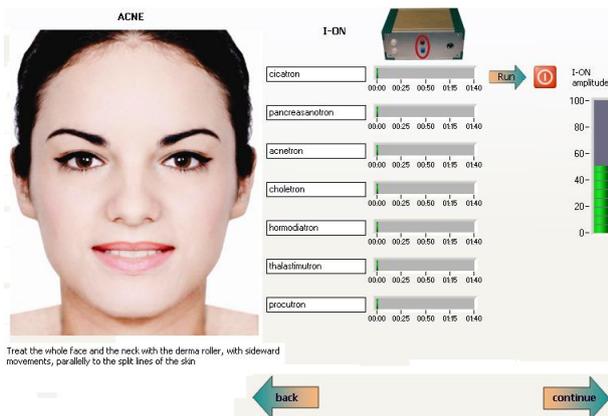


Treat the whole face and the neck with the derma roller, with sideward movements, parallelly to the splk lines of the skin

FACIAL ACNE TREATMENT WITH THE i-ON:

- Client in supine position
- Attach the (red) 0-electrode to the wrist
- Adjust the proper current amplitude
- Click the “run”-arrow to activate the first 2 Raymedies
- Treat the whole face with the dermaroller
- Interrupt thereafter, remove the remains of Aloe+Restorate, and apply a new mask with Aloe+Q10
- Continue the protocol
- Remove the remaining Aloe-mixture
- Click “continue” to move on when finished

5.5.4 FACIAL ACNE TREATMENT WITH THE I-VAC

Due to the damaged skin situation, the only aim of facial cupping is improving the detoxification and circulation by lymph drainage

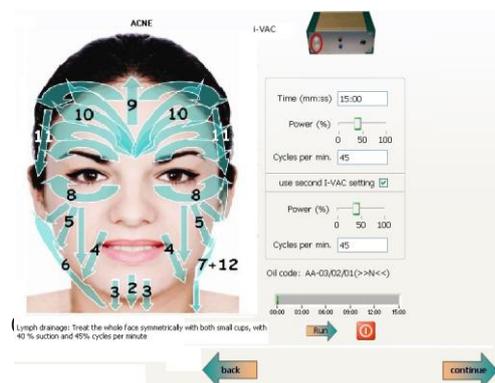

Lymph drainage: Treat the whole face symmetrically with both small cups, with 40 % suction and 45% cycles per minute


FACIAL ACNE TREATMENT WITH THE i-VAC:

- Client in supine position
- Mix almond oil with the elemental oil complex as indicated on screen
- Follow further screen indications

- **Lymph drainage**

1. In the clavicular groove (acupuncture point St11): 7-8 suction cycles
2. From the center of the lower lip across the lower edge of the chin
3. With both cups from the lower lip across the lower edge of the chin
4. From the nasolabial wrinkle across the lower edge of the chin (see picture)
5. From the cheeks across the lower edge of the chin (see picture)
6. From the middle lower edge of the chin sideward to a depression below the ear lobes (acupuncture point TH 17)
7. From 3H17 to the clavicular groove (St11): 7-8 suction cycles
8. From the inner eye corner to the outer eye corner (Tai Yang)
9. From Yin Tang (between the eye brows) to the hair border
10. From the forehead center across the temporal area to Tae Yang: 3-4 suction cycles
11. From Tae Yang to the depression below the ear lobe (TH17): 3-4 suction cycles
12. From there to the clavicular groove (St11) 7-8 suction cycles

5.5.4 FACIAL ACNE TREATMENT WITH THE I-LIGHT

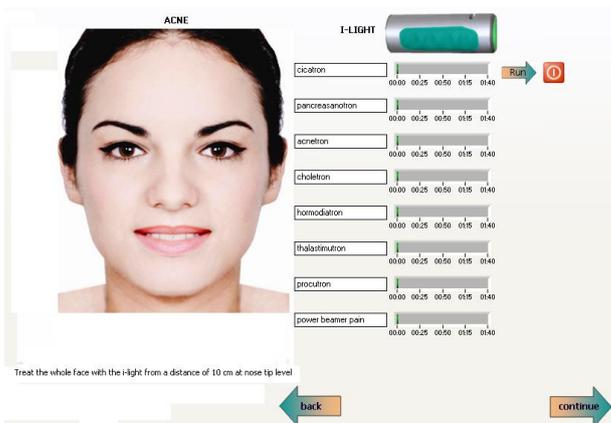

FACIAL ACNE TREATMENT WITH THE i-LIGHT:

- Client in supine position
- Remove the remaining oil, and activate the Raymedies by clicking the “run”-arrows next to the Raymedies on screen
- Beam the i-Light to the face at nose tip level, at a 10 cm distance

Please do 1 EDA measurement for the i-health skin analysis.

1366	Lo 11	2269
1369	Di 1	2409
1625	C 9	2465
2281	3E 1	2405
2327	H 9	2400
2353	Du 1	2363
2354	MP 1	2378
2411	Le 1	2364
2403	M 45	2423
2404	G 44	2440
2422	N 1	2458
2434	B 67	2301

NEW EDA MEASUREMENT

- A next EDA measurement is necessary, preceding the concluding consolidation stage
- Follow the instructions on screen
- When finished, click “continue” to move on

5.5.3 FINAL STAGE ACNE PROGRAM:CONSOLIDATION WITH THE RED BEAMER

Beamer
EARTH Hypo, Heart
emochacratron 4

00:00 00:25 00:50 01:15 01:40 Run

ACNE

Apply the beamer on the belly button

CONSOLIDATION STAGE

- Client in supine position
- According to the actual energy depletion in the Earth element, as mentioned in this example, the program selects automatically the Raymedy Eموchacratron 4: energy supply from the Fire Element.
- Apply the red Beamer to the navel, and activate the Raymedy by clicking the “run”-arrow

After having clicked the “continue”-arrow, the acne program will be finished and closed:

Protocoll is finished.

5.6 CELLULITE PROGRAM

For practical topographic reasons, Cellulite in this program has been subdivided into 3 forms, due to the correlation with the concerned meridians:


G/liv, (Gallbladder/Liver), SP/St (Spleen-Pancreas-Stomach), en K/B (Kidney/Bladder)

G/Liv cellulite will be treated with the client laying on the right or left side, SP/St cellulite in supine position, and K/B cellulite in prone position, Because the SP/St function plays an important role in all kinds of cellulite, it is recommended to combine the SP/St meridians/zones with each cellulite treatment.

During performing the Cellulite programs, pictures will be shown with the cellulite zones, the dermatomes, the shu points and the alarm points.

3 EDA measurements define the client's constitutional energy type (normal, hypo-, or hyper)

After having selected the cellulite program in general, 3 types of cellulite will appear on your screen:

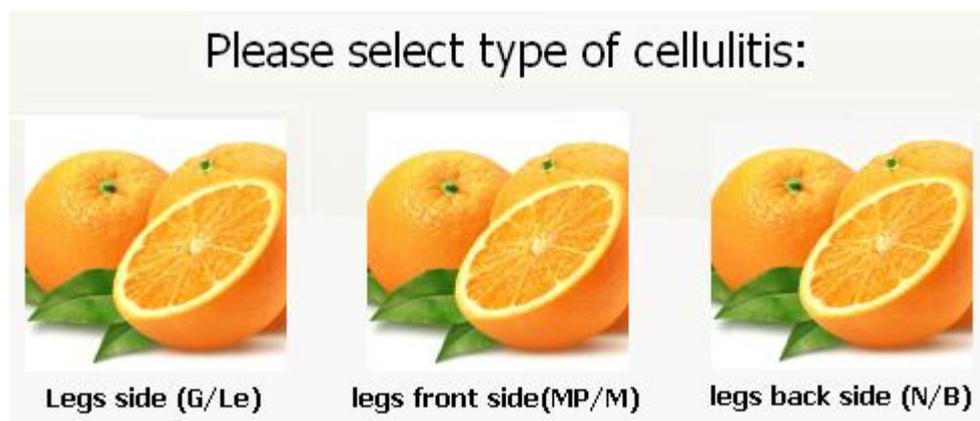


All cellulite programs will provide a cellulite treatment of the legs in particular, and contain a similar construction. There is only a differentiation concerning the specific treatment zones. That's why only the G/Liv program will be described in detail.

5.6.1 CELLULITE PROGRAM G/LIV (LATERAL SIDE OF LEGS)



3 preceding EDA measurements are necessary to define the client's element type, the amount of energy, the regulative capacity, the energy distribution and the weakest meridian. As a result, the next screen will indicate the proper direction of movement with the vacuum cups with the personal essential oil complex.

7.6.2 CELLULITE PROGRAM G/LIV. BACK TREATMENT WITH THE I-VAC

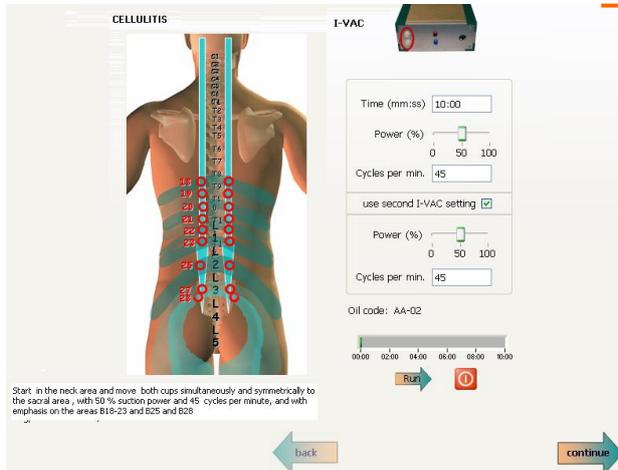


CELLULITE: BACK TREATMENT WITH THE I-VAC

- Client in prone position
- Follow the instructions on screen
- Activate the i-VAC by clicking the “run”-arrow
- The proper vacuum power and pulsations have been preprogrammed, but can be adapted
- Move both big vacuum cups symmetrically and simultaneously in the indicated direction along the spine, and emphasize the marked points with 7-8 extra suction pulses
- Remove the oil remains when you are finished with the i-VAC
- Click the “continue”-arrow to move on

5.6.3 CELLULITE PROGRAM G/LIV. TREATMENT OF THE PROBLEMATIC ZONES WITH THE I-ON


The treatment described here should be repeated with the other leg

- Start with 10 min. infrared radiation on the problematic tissue zones
- Apply the Aloe+Restorate mix on the lateral problematic zones of one leg
- Radiate these zones with I-LIGHT (white light)
- Start the i-ON treatment with the dermaroller with Cicatron and Basetron
- After that, interrupt the Raymedy supply, remove the Aloe-Restorate mixture and replace it with Aloe+CC Cell lotion+Cinnamon+Activize
- To enhance the warming effect, the upper leg is wrapped in cellophane foil
- **Repeat this i-LIGHT- and i-ON procedure with the other leg**

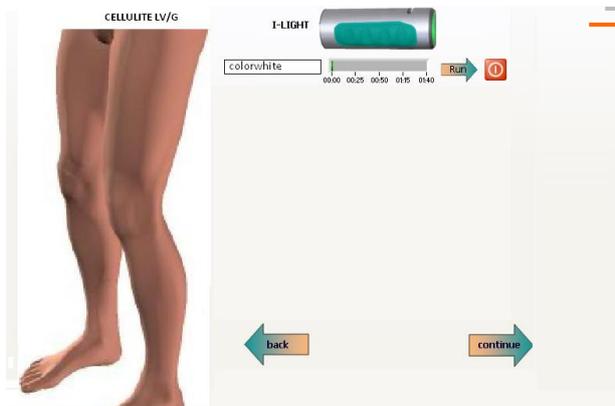

CELLULITE: i-ON PREPARATION WITH THE i-LIGHT

- Client on the right or left side
- Apply the Aloe+Restorate mix on the lateral problematic zones
- Click the “run”-arrow to activate the i-LIGHT
- Beam the i-LIGHT to the leg, at a 10 cm distance
- Click the “Continue”-arrow to move on

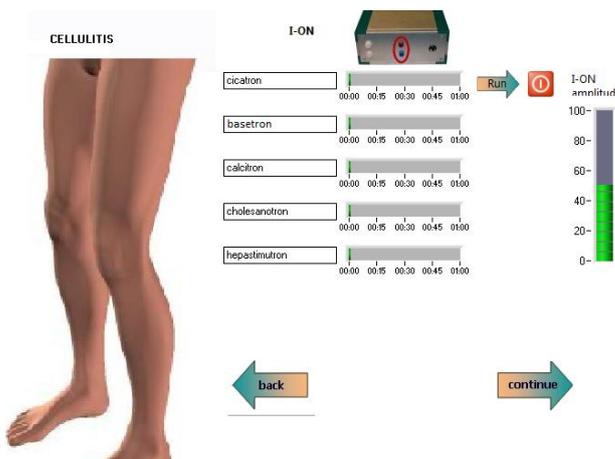

CELLULITE: LEG TREATMENT WITH THE i-ON

- client on the right or left side
- Adjust the proper current amplitude
- Activate the i-ON by clicking the “run”-arrow
- after Cicatron and Basetron, replace the Aloe + restorate mix with Aloe + CC Cell lotion + Cinnamon + Activize and continue the i-ON treatment
- When finished, wrap the upper leg in cellophane foil and repeat this i-ON procedure with the other leg

5.6.4 CELLULITE PROGRAM G/LIV. TREATMENT OF THE PROBLEMATIC ZONES WITH THE I-VAC

Unwrap the first leg, and remove carefully the Aloe-CC Cell-Activize-Cinnamon mixture with a warm moisturized towel. Apply the proper Almond oil – 5 elements-combination to the zones to be treated.

I-VAC LYMPHE DRAINAGE


Activate the i-Vac by clicking the “run” arrow. Start with one small vacuum cup:

- In the clavicular groove (acupuncture point St11): 7-8 suction cycles
- Between the big toe and the 2nd toe (acupuncture point Liv 3): 7-8 suction cycles
- Exchange the small vacuum glass for the big one:
 - Move the big cup from the outer side of the upper leg to the inner side
 - 7-8 suction cycles at Liv 8 (inner side of the knee), and move back to the outer side of the upper leg
 - Treat that outer side with both big cups, from the knee area to the hip area
 - Adjust the suction power according to your clients sensitivity

I-VAC CONNECTIVE TISSUE MASSAGE

- Change the cycle velocity to 550, and diminish the vacuum power to at least 25 %
- Work with just one vacuum cup superficially but rather fast on the same area as before, from the knee to the hip area
- Remove the oil remains carefully with a warm moisturized towel


Repeat the same procedure with the other leg

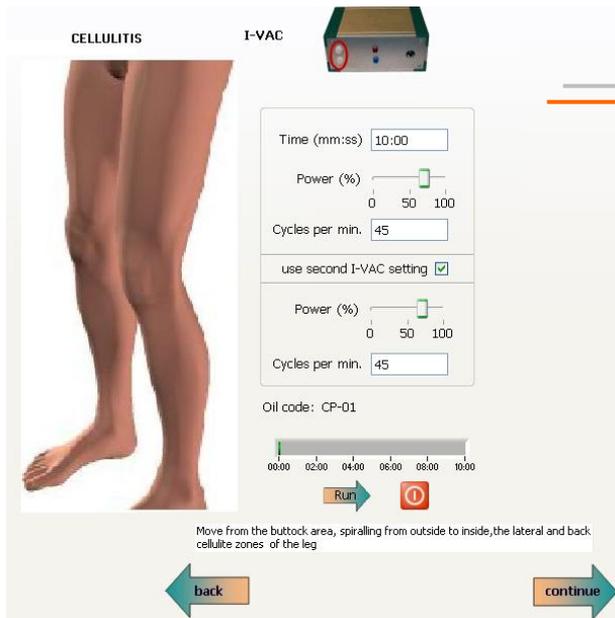

CELLULITE: LEG TREATMENT WITH THE I-VAC

- Client laying on left or right side
- Follow the instructions on screen
- Activate the i-VAC by clicking the “run”-arrow
- The proper vacuum power and pulsations have been preprogrammed
- Click the “continue”-arrow to move on when finished with the i-VAC

5.6.5 CELLULITE PROGRAM G/LIV. TREATMENT OF THE PROBLEMATIC ZONES WITH THE I-LIGHT

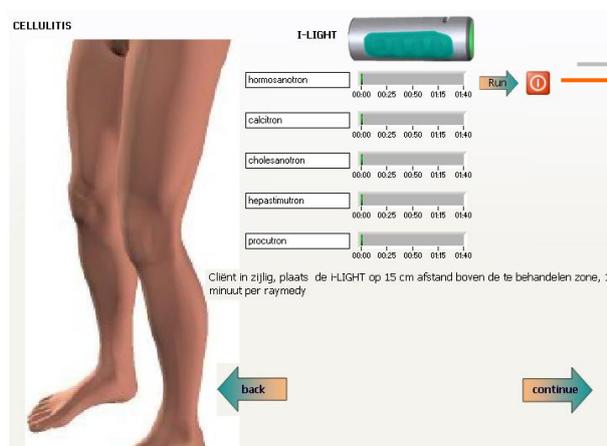

CELLULITE: LEG TREATMENT WITH THE I-LIGHT

- Client laying on left or right side
- Follow the instructions on screen
- Activate the i-LIGHT by clicking the “run”-arrow
- Click the “continue”-arrow to move on when finished with the i-LIGHT


5.6.6 CELLULITE PROGRAM G/LIV. ABDOMINAL TREATMENT WITH THE I-VAC

Apply a warmed oil-combination to the abdominal area. Activate the i-VAC by clicking the ‘run’-arrow, adjust the suction power according to your client’s sensitivity.

Start with both big cups simultaneously at the left and right side of the abdomen and move as indicated to the belly centre, move them back to both sides, follow from there the upper arrows to the


gastric area, back again, then follow the lower arrows to the pubic area. Finally, follow the indicated arrow direction along the Conception Vessel (Ren Mai)

Remove the oil remains carefully with a warm moisturized towel, and continue for the next step

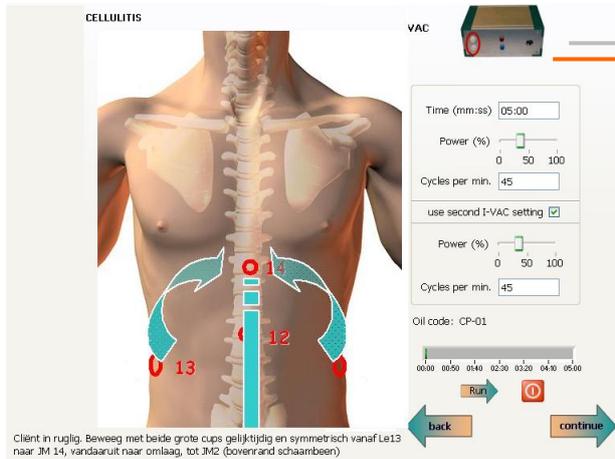

CELLULITE: ABDOMINAL TREATMENT WITH THE I-VAC


- Client in supine position
- Follow the instructions on screen
- Activate the i-VAC by clicking the “run”-arrow
- The proper vacuum power and pulsations have been preprogrammed
- Click the “continue”-arrow to move on when finished with the i-VAC

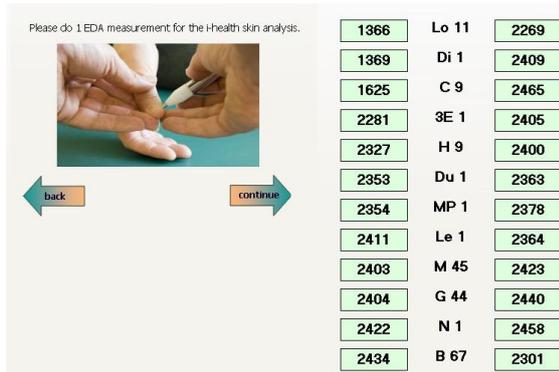

NEW EDA-MEASUREMENT

- To proceed the concluding consolidation stage, a new EDA measurement is necessary
- Follow the instructions on screen

5.6.7 CELLULITE PROGRAM G/LIV: CONSOLIDATION WITH THE RED BEAMER

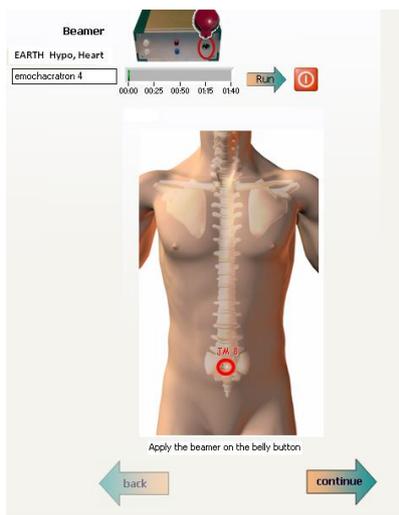

CONSOLIDATION STAGE

- Client in supine position
- Due to the actual energy depletion in the client’s constitutional Earth element, the program selects in this example automatically the Raymedy Emochacratron 4: energy supply from the Fire Element
- Apply the red beamer to the navel, and activate the Raymedy by clicking the “run”-arrow

By clicking the “continue”-arrow after having finished the consolidation stage, the cellulite program will be closed and your screen will show the text:

Protocoll is finished.

QUICKVIEW CELLULITE PROGRAMS MP/S AND K/B

Adjustment only for Cellulite treatments at the front and back of the legs

1. 8 min. infrared radiation on the problematic tissue zones
2. 3 EDA measurements
3. Lymph drainage according to protocol
4. Application with Aloe+Restorate on the problematic zones of one of both legs (front or back)
5. I-LIGHT with white light
6. i-ON with the dermaroller with Acidiatron
7. Remove the remains of Aoe + Restorate, continue i-ON with Aloe+ CC-Cell Lotion (ratio 1:2), do not remove these remains

8. Application with Aloe+Restorate on the problematic zones of the other leg (front or back)
9. I-LIGHT with white light
10. i-ON with the dermaroller with Acidiatron
11. Remove the remains of Aoe + Restorate, continue i-ON with Aloe+ CC-Cell Lotion (ratio 1:2), do not remove these remains

12. Clean the first treated leg with a hot towel
13. I-VAC according to protocol with almond oil + 5 elements CPL

14. Clean the second treated leg with a hot towel
15. I-VAC according to protocol with almond oil + 5 elements CPL

16. Remove the remains of the almond oil mixture from both legs
17. I-LIGHT according to protocol

18. Lymph drainage of the abdomen


19. EDA measurement

20. Beamer Emochakraton

5.7 SPECIAL SOLUTIONS

Programs for several specific skin and beauty problems are under construction right now. This chapter contains a typical ‘demo-protocol”, which allows beauty practitioners to get their new and interested clients acquainted with all effective ingredients of the Energy Skin Care Module.


5.7.1 DEMO PROGRAM-BACK TREATMENT WITH THE I-ON, I-VAC AND I-LIGHT

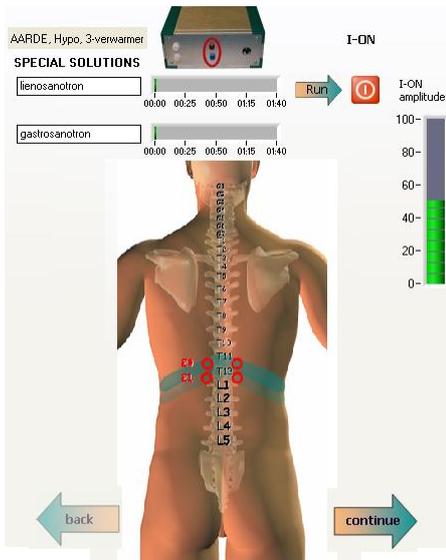

Beweeg met de dermaroller vanuit het midden naar links en rechts

DEMO-PROGRAM: i-ON BACK TREATMENT


- Adjust the proper current amplitude
- Click the “run”-arrow to activate the i-ON
- Follow the instructions on screen
- Click the “continue”-arrow to enter the next step

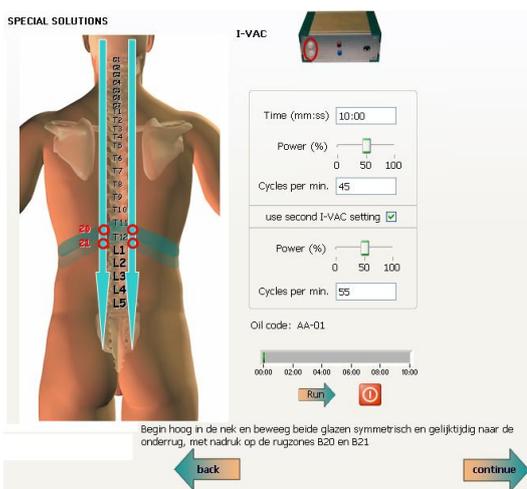

Begin hoog in de nek en beweeg beide glazen symmetrisch en gelijktijdig naar de onderrug, met nadruk op de rugzones B20 en B21

DEMO-PROGRAM: i-VAC BACK TREATMENT

- Client in prone position
- Follow the instructions on screen
- Activate the i-VAC by clicking the “run”-arrow
- The proper vacuum power and pulsations have been preprogrammed
- Click the “continue”-arrow to move on when finished with the i-VAC

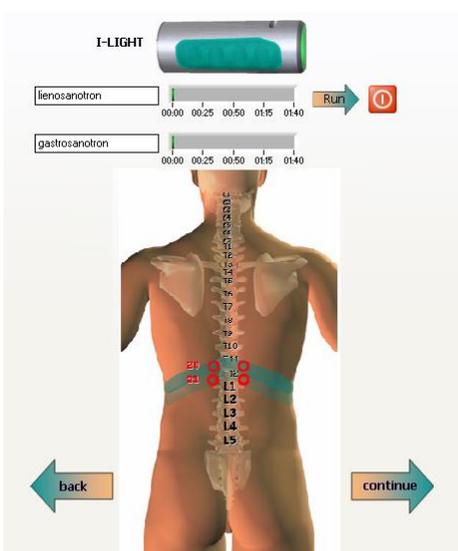

Richt de I-LIGHT achtereenvolgens tussen de punten B20 en B21


DEMO-PROGRAM: i-LIGHT BACK TREATMENT

- Click the “run”-arrow to activate the i-LIGHT
- Follow the instructions on screen
- Click the “continue”-arrow to enter the next step

5.7.2 DEMO PROGRAM-FACIAL TREATMENT WITH THE I-ON, I-VAC AND I-LIGHT


Prepare two mixtures: one mixture of Aloe+Restorate, another one of Aloe+Q10+Rebuild25.

Clean the face with rose water. Then, apply a facial mask of Aloe+Restorate and radiate the face with white light from the i-LIGHT. Ask the client to keep the eyes closed during this procedure.

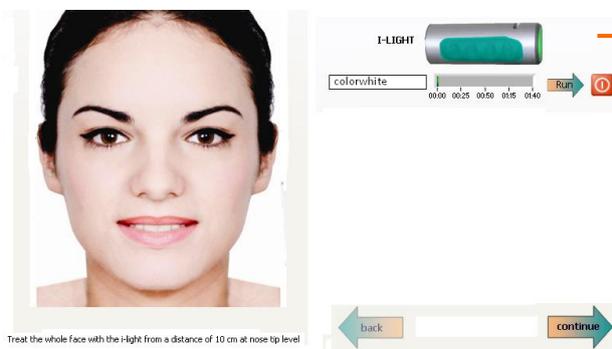

i-LIGHT PREPARATION PRECEDING I-ON TREATMENT:

- Client in supine position, with eyes closed
- Beam the i-LIGHT to the face, at a 10 cm distance
- Click “run” to activate the i-LIGHT
- Click the “Continue”-arrow to move on

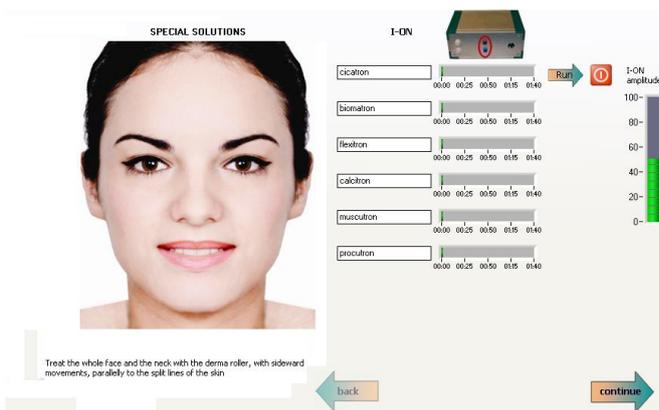


DEMO-PROGRAM: i-ON FACIAL TREATMENT

- Apply contact gel
- Adapt current amplitude to a sub-sensitive level
- Activate Raymedies by clicking on the “run” –arrow
- Connect Dermaroller to red i-Matrix socket
- Connect 0-electrode to black i-Matrix socket
- Treat indicated dermal zones with the dermaroller
- Click “continue” arrow to enter the next step




DEMO-PROGRAM: i-VAC FACIAL TREATMENT

- Client in supine position
- Remove the remaining contact gel, and mix almond oil with the elemental oil complex as indicated on screen
- Follow further screen indications
- Click "continue" arrow to enter the next step

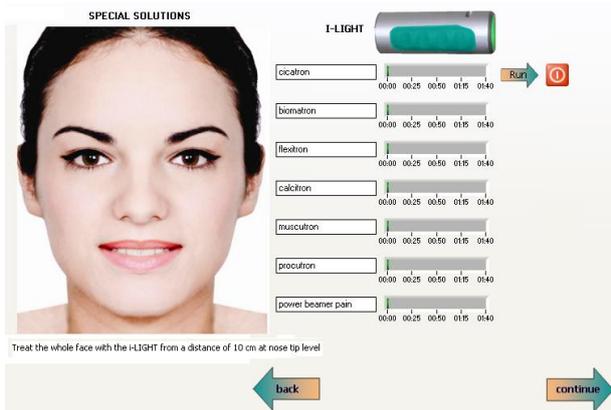

DEMO-PROGRAM: i-LIGHT FACIAL TREATMENT


- Client in supine position
- Remove the remaining oil, and activate the Raymedies by clicking the "run"-arrows next to the Raymedies on screen
- Beam the i-Light to the face at nose tip level, at a 10 cm distance
- Click "continue" arrow to enter the next step

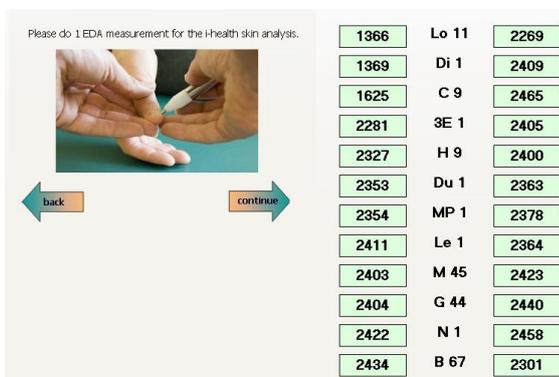

NEW EDA MEASUREMENT

- A next EDA measurement is necessary, preceding the concluding consolidation stage
- Follow the instructions on screen
- When finished, click "continue" to move on

5.7.3 DEMO PROGRAM-CONSOLIDATION STAGE WITH THE RED BEAMER

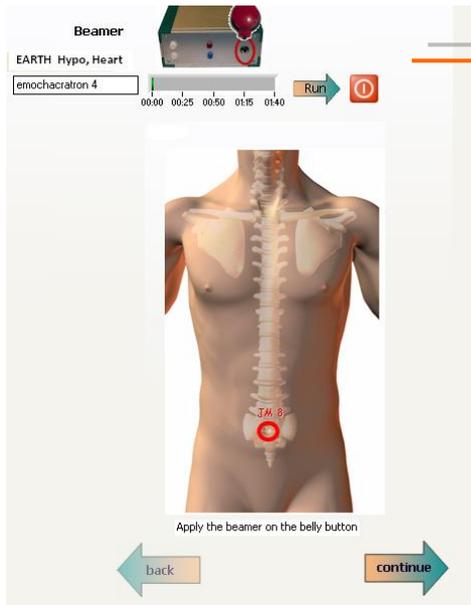

DEMO PROGRAM FINAL STAGE - CONSOLIDATION

- Client in supine position
- Due to the actual energy excess in the Earth Element (in this example) , automatically the program has selected the Raymedy Emodacatron 5: discharge of energy excess to Metal
- Apply the red beamer to the navel, and activate the Raymedy by clicking the “run”-arrow

This demo-program will be closed after having clicked the “continue”-arrow. You will read on screen the text:

Procoll is finished.